
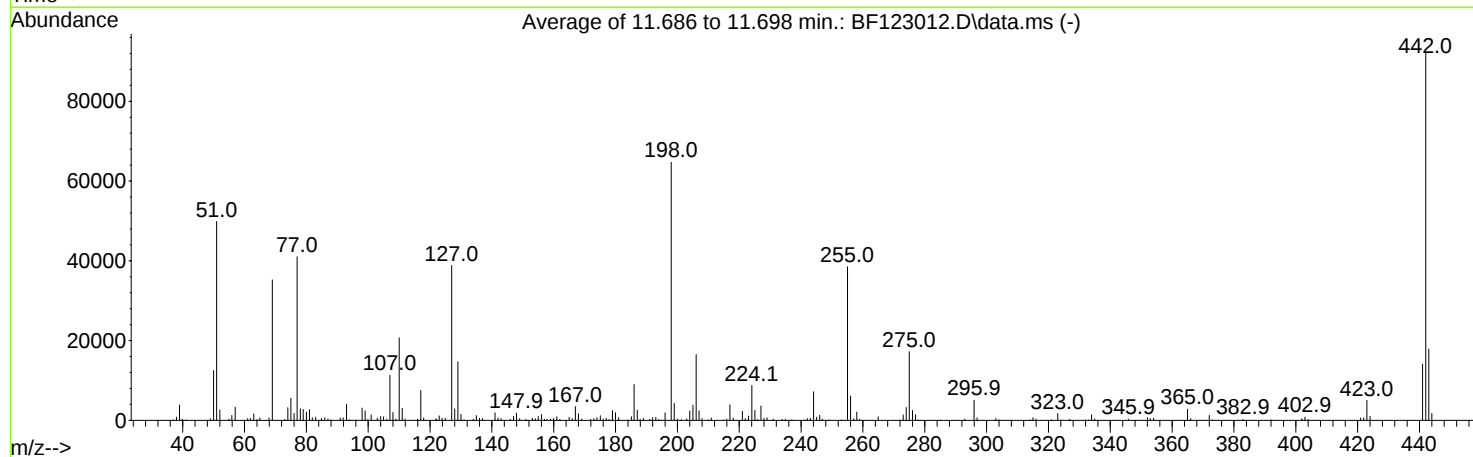


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011921\
 Data File : BF123012.D
 Acq On : 19 Jan 2021 10:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 18 13:14:08 2021

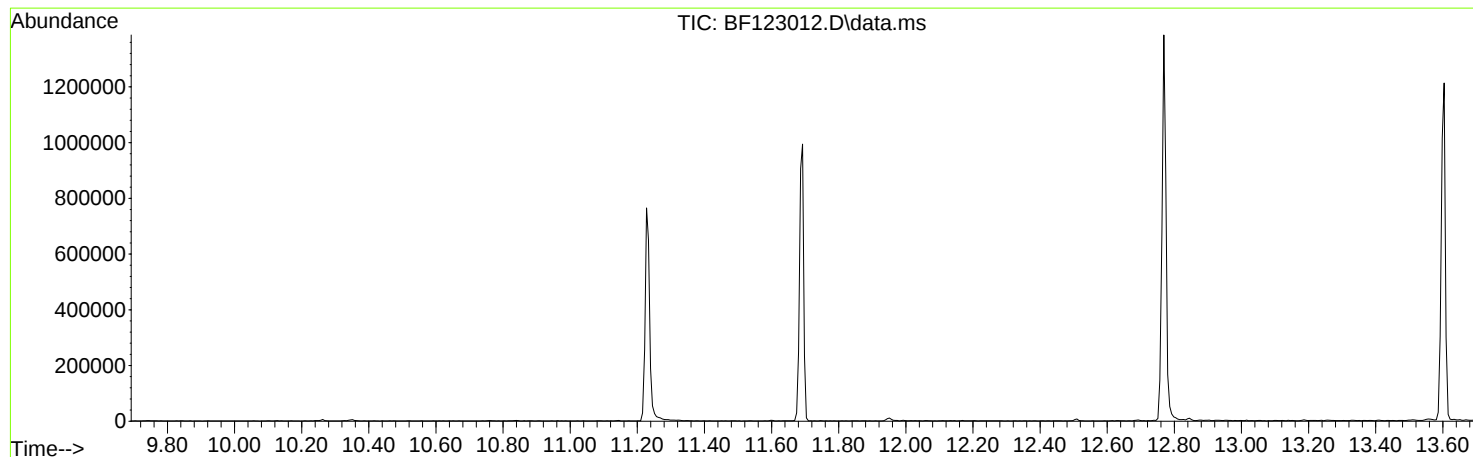

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	77.1	49882	PASS
68	69	0.00	2	1.7	592	PASS
69	198	0.00	100	54.4	35207	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	60.0	38842	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64696	PASS
199	198	5	9	6.6	4240	PASS
275	198	10	60	26.6	17222	PASS
365	198	1	100	4.3	2794	PASS
441	198	0.01	100	21.8	14084	PASS
442	442	50	100	100.0	92229	PASS
443	442	15	24	19.4	17855	PASS