


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011924\
Data File : BF137106.D
Acq On : 19 Jan 2024 12:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 20 00:58:12 2024

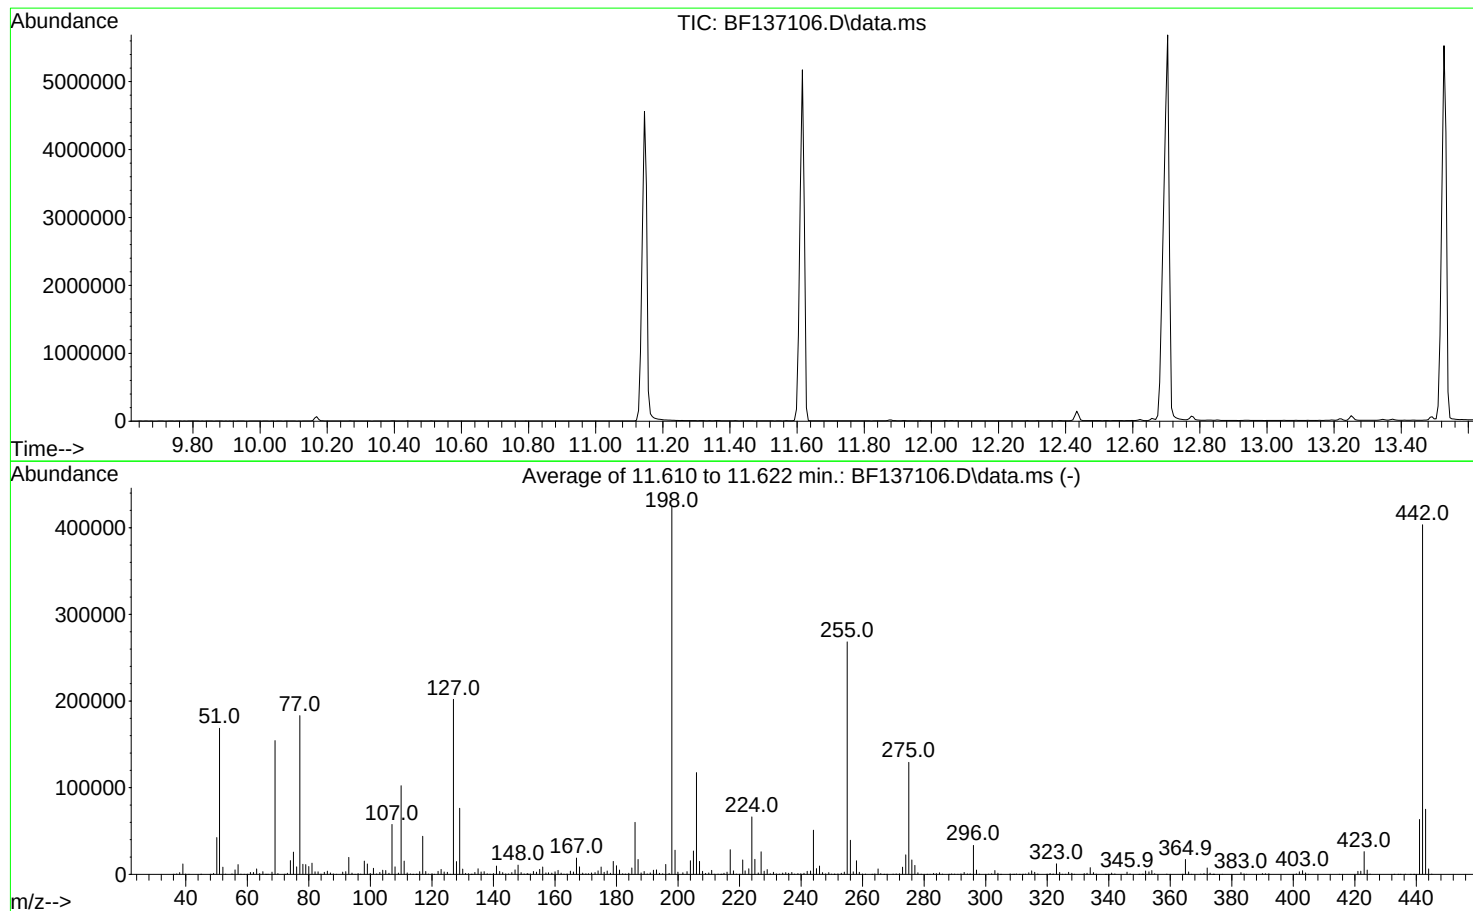




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	168557	PASS
68	69	0.00	2	1.7	2584	PASS
69	198	0.00	100	36.4	154312	PASS
70	69	0.00	2	0.6	879	PASS
127	198	10	80	47.6	201941	PASS
197	198	0.00	2	0.3	1099	PASS
198	198	100	100	100.0	424491	PASS
199	198	5	9	6.6	27813	PASS
275	198	10	60	30.5	129320	PASS
365	198	1	100	4.0	17145	PASS
441	198	0.01	100	14.9	63341	PASS
442	442	50	100	100.0	403477	PASS
443	442	15	24	18.6	75163	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011924\
Data File : BF137106.D
Acq On : 19 Jan 2024 12:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 20 01:06:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 20 00:58:12 2024
Response via : Initial Calibration

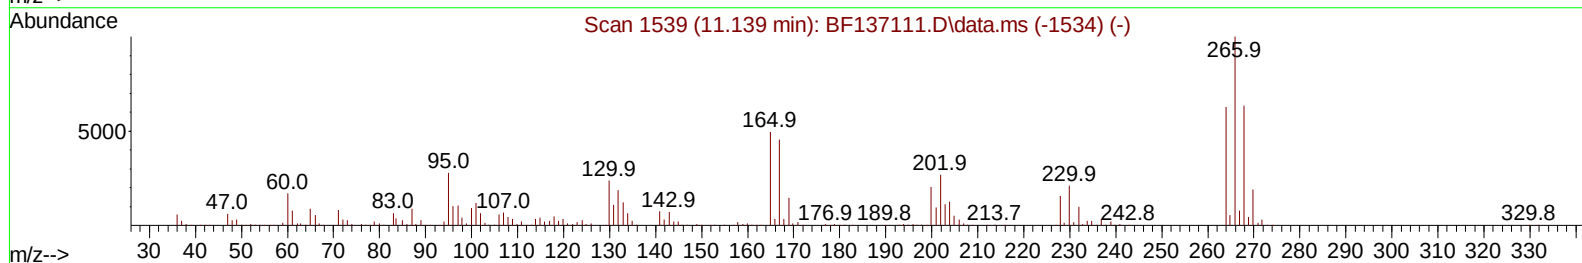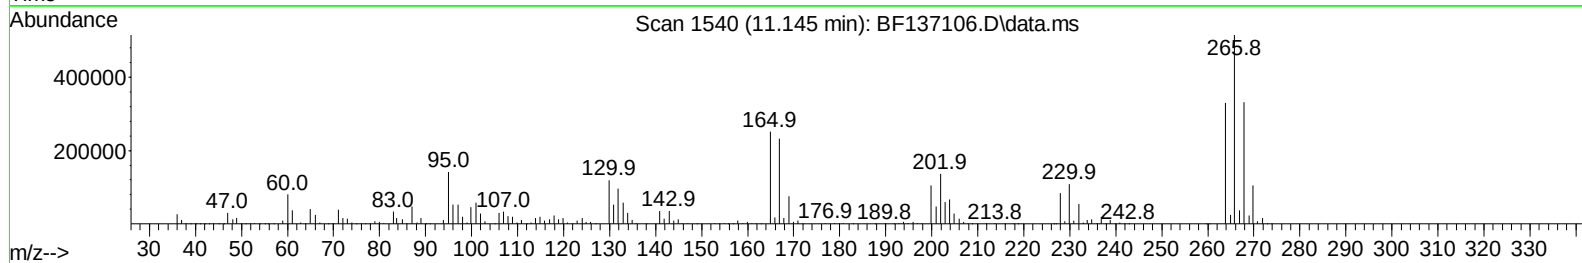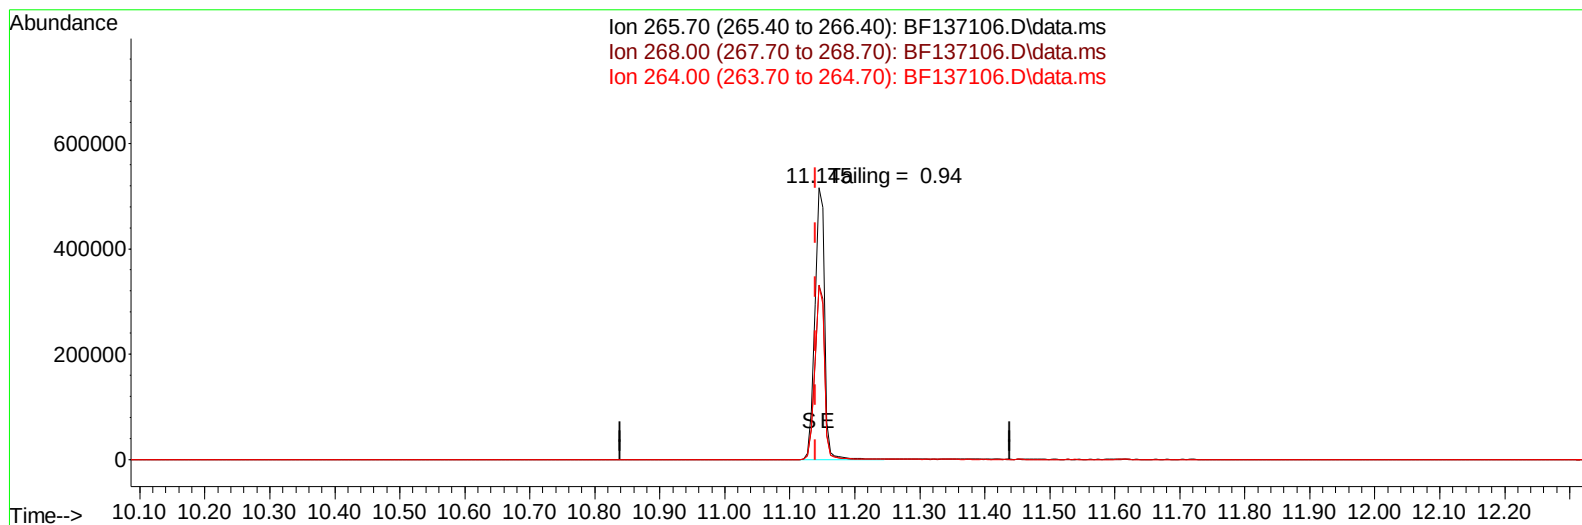

TIC: BF137106.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.006) 188235.40 ng




response 535950

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	64.27
264.00	62.60	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011924\
Data File : BF137106.D
Acq On : 19 Jan 2024 12:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 20 01:06:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 20 00:58:12 2024
Response via : Initial Calibration

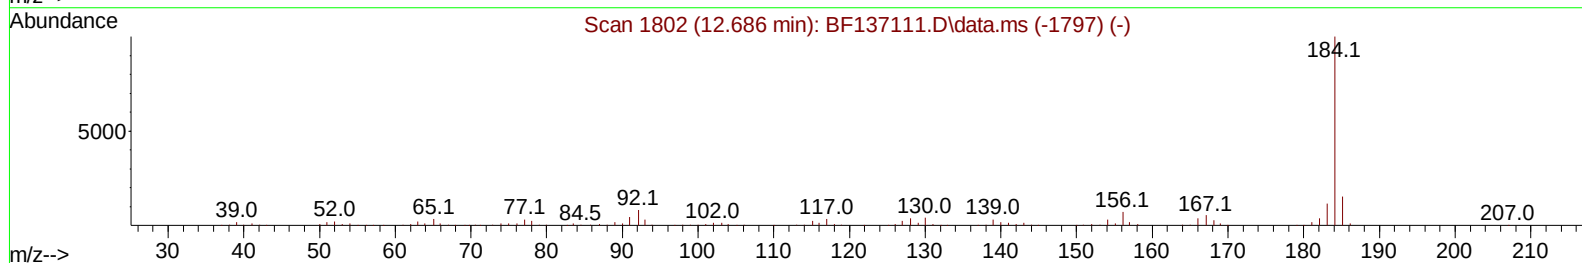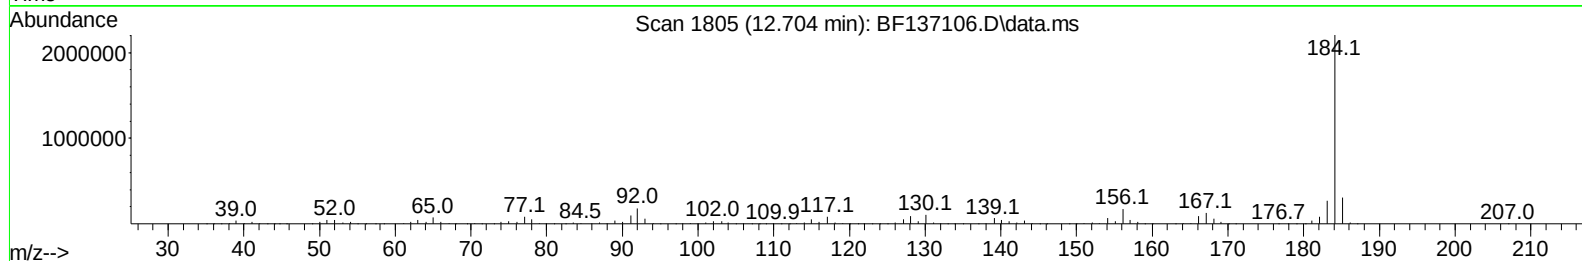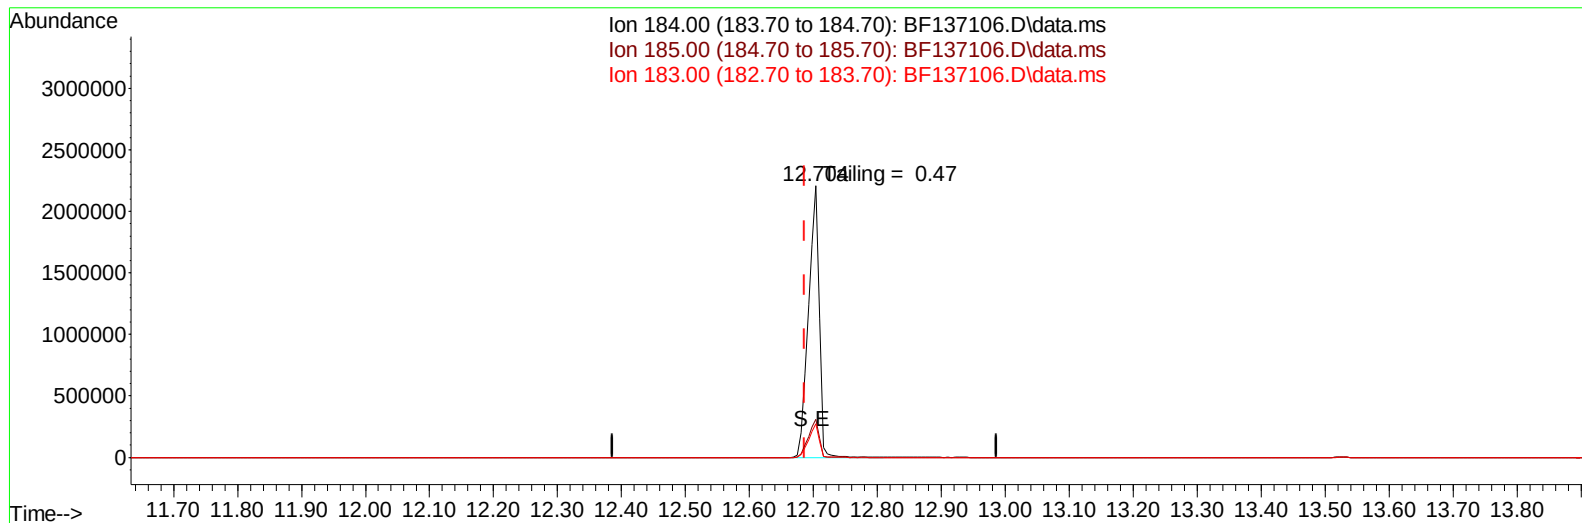

TIC: BF137106.D\data.ms

(77) Benzidine

12.704min (+ 0.018) 593539.44 ng

response 2618338

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.07
183.00	11.50	12.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/19/2024	BNA_F	<u>BF137106.D</u>
Compound Name	Response	Retention Time
DDT	969591	13.527
DDD	12155	13.251
DDE	72	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12227	981818	1.25

Instrument :
BNA_F
ClientSampleId :
DFTPP