


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012015\
 Data File : BF076960.D
 Acq On : 20 Jan 2015 12:49
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 21 11:38:13 2015

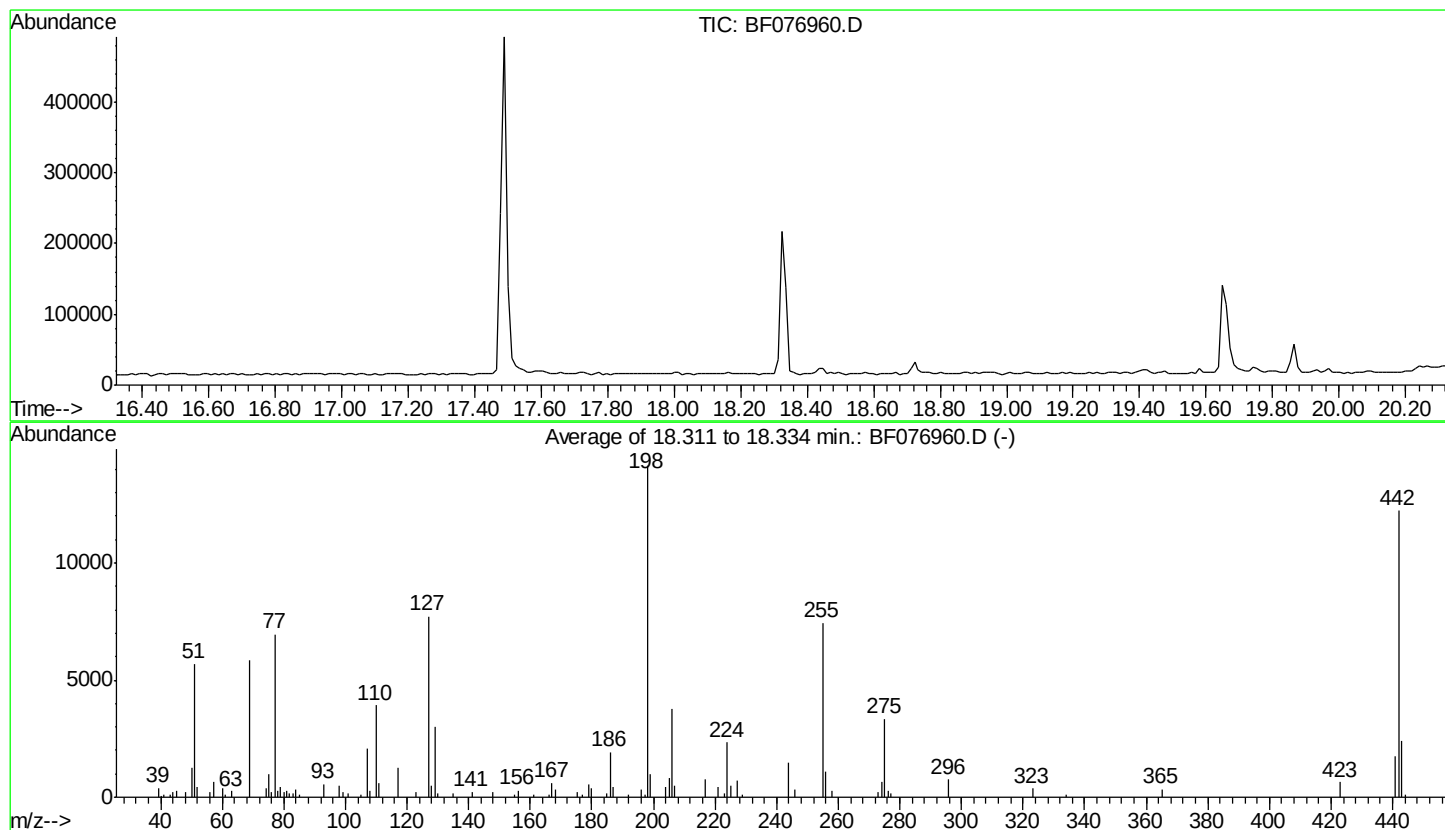

AutoFind: Scans 1507, 1508, 1509; Background Corrected with Scan 1504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	5694	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.3	5842	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.5	7709	PASS
197	198	0.00	2	0.7	103	PASS
198	198	100	100	100.0	14154	PASS
199	198	5	9	6.8	962	PASS
275	198	10	60	23.7	3348	PASS
365	198	1	100	2.5	348	PASS
441	442	0.01	24	14.4	1761	PASS
442	198	50	100	86.3	12215	PASS
443	442	15	24	19.6	2395	PASS