
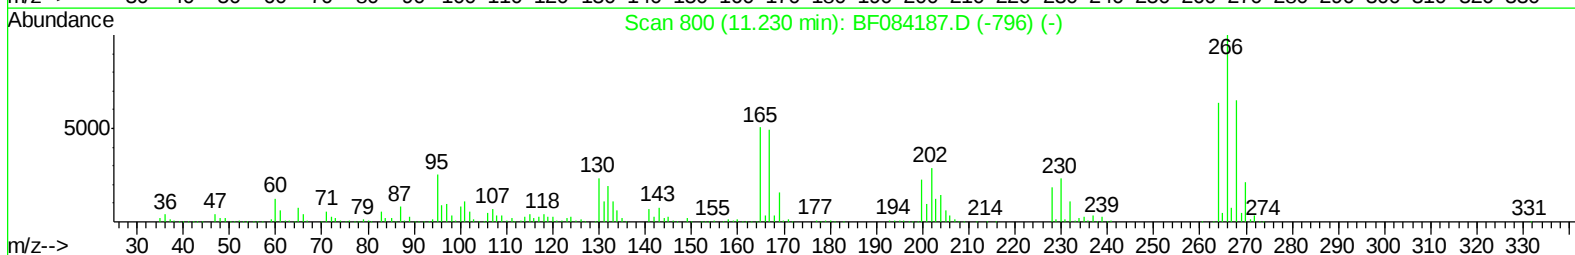
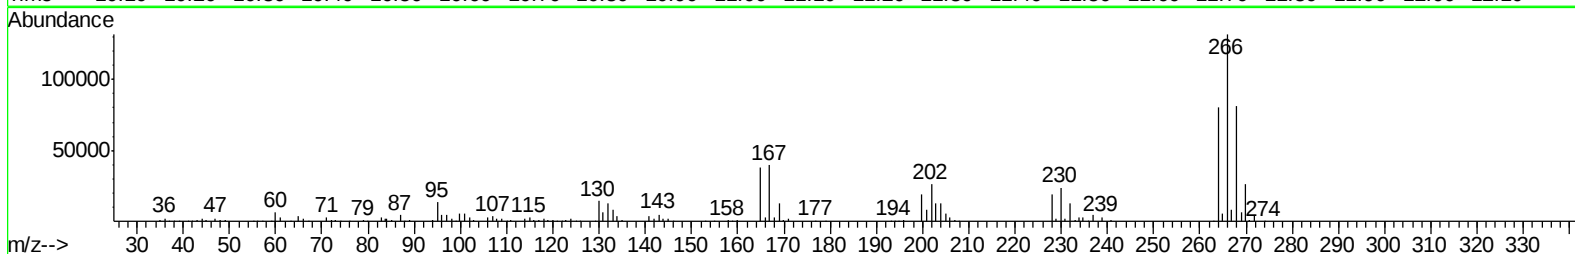


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF012016\  
Data File : BF084562.D  
Acq On : 20 Jan 2016 9:39  
Operator : SJ/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 07:34:08 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF123115.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jan 14 14:15:52 2016  
Response via : Initial Calibration

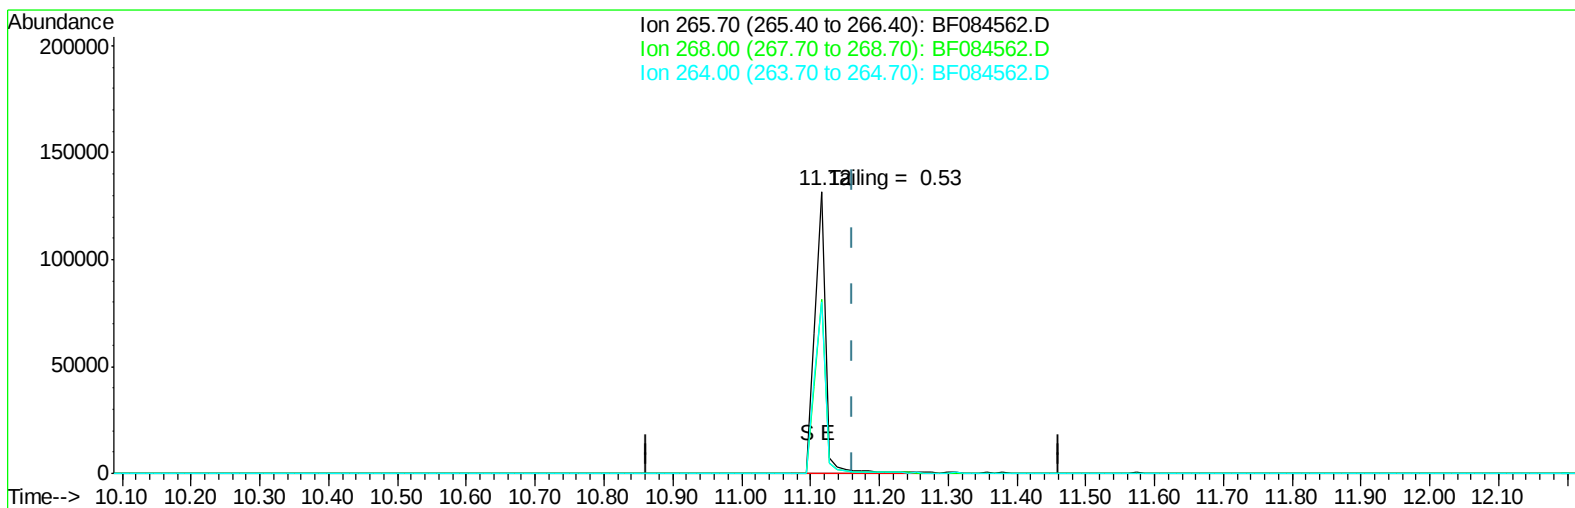

TIC: BF084562.D

(69) Pentachlorophenol (C)




11.116min (-0.046) 22597.26ng

response 147195

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.50 | 61.67 |
| 264.00 | 62.70 | 61.12 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF012016\  
Data File : BF084562.D  
Acq On : 20 Jan 2016 9:39  
Operator : SJ/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 07:34:08 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF123115.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jan 14 14:15:52 2016  
Response via : Initial Calibration

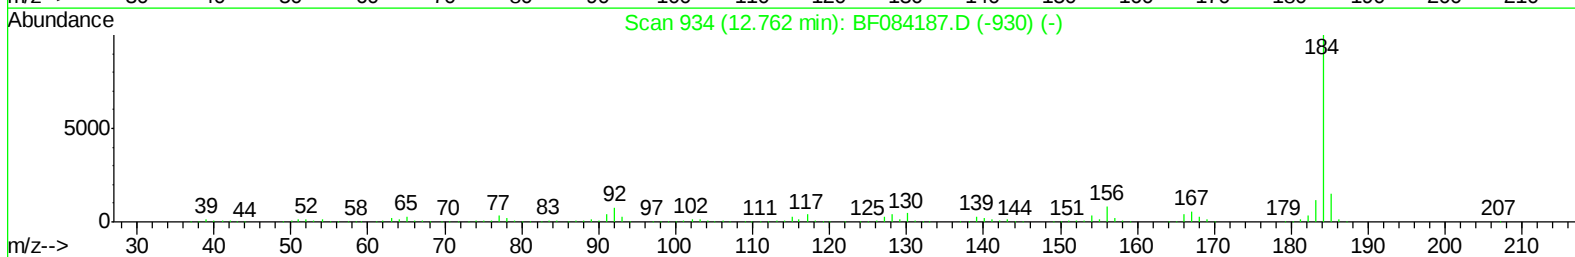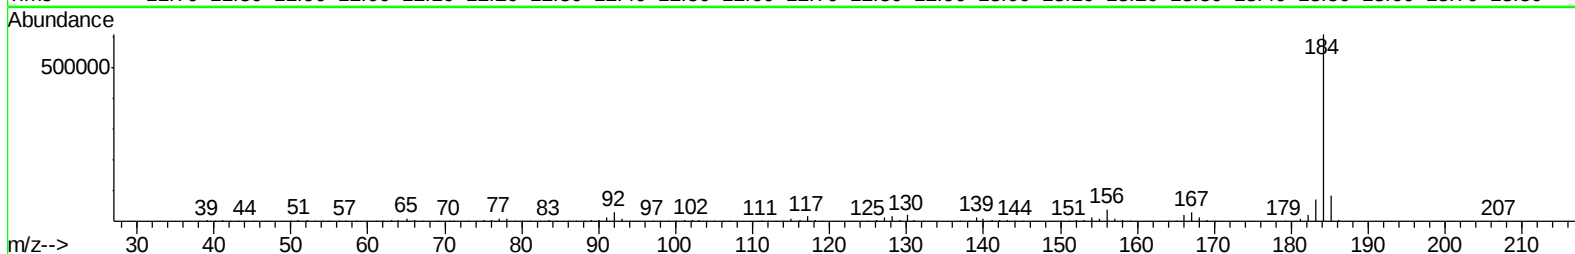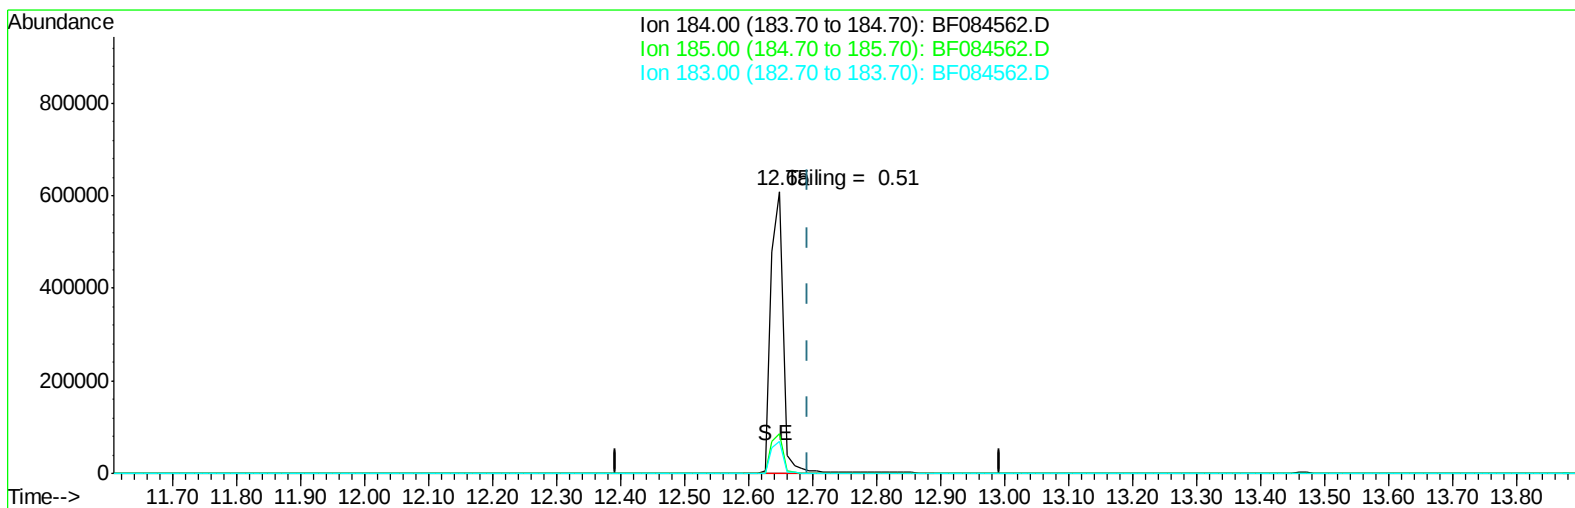

TIC: BF084562.D

(76) Benzidine

12.648min (-0.046) 9849.62ng

response 828157

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.20 | 13.93 |
| 183.00 | 12.30 | 11.53 |
| 0.00   | 0.00  | 0.00  |