


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012016\
Data File : BF084562.D
Acq On : 20 Jan 2016 9:39
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 14 14:15:52 2016

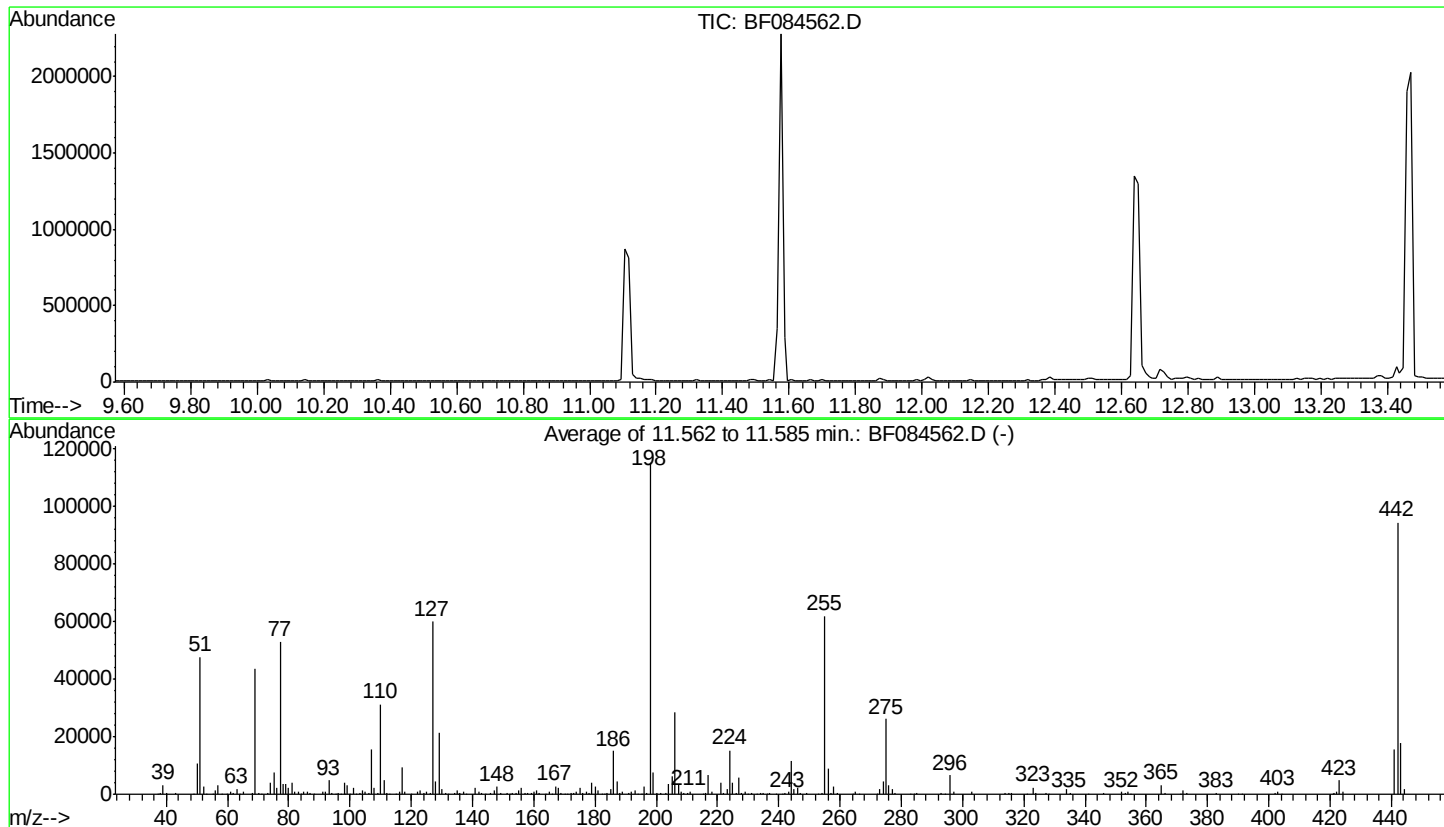

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	47600	PASS
68	69	0.00	2	1.4	618	PASS
69	198	0.00	100	37.9	43713	PASS
70	69	0.00	2	0.8	335	PASS
127	198	10	80	52.1	59967	PASS
197	198	0.00	2	0.5	534	PASS
198	198	100	100	100.0	115186	PASS
199	198	5	9	6.6	7589	PASS
275	198	10	60	22.6	26075	PASS
365	198	1	100	2.7	3148	PASS
441	442	0.01	24	16.4	15476	PASS
442	198	50	100	81.9	94352	PASS
443	442	15	24	18.9	17838	PASS