
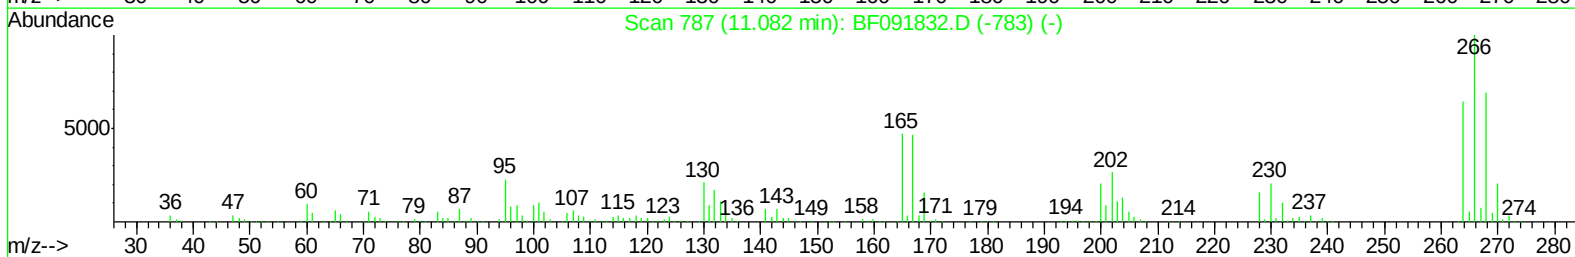
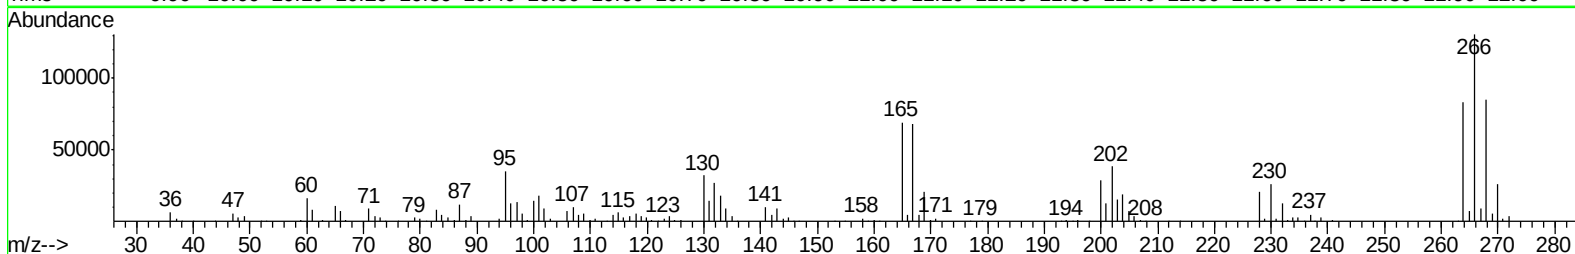


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012017\
Data File : BF092365.D
Acq On : 20 Jan 2017 10:51
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 07:27:44 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 23 01:12:17 2017
Response via : Initial Calibration

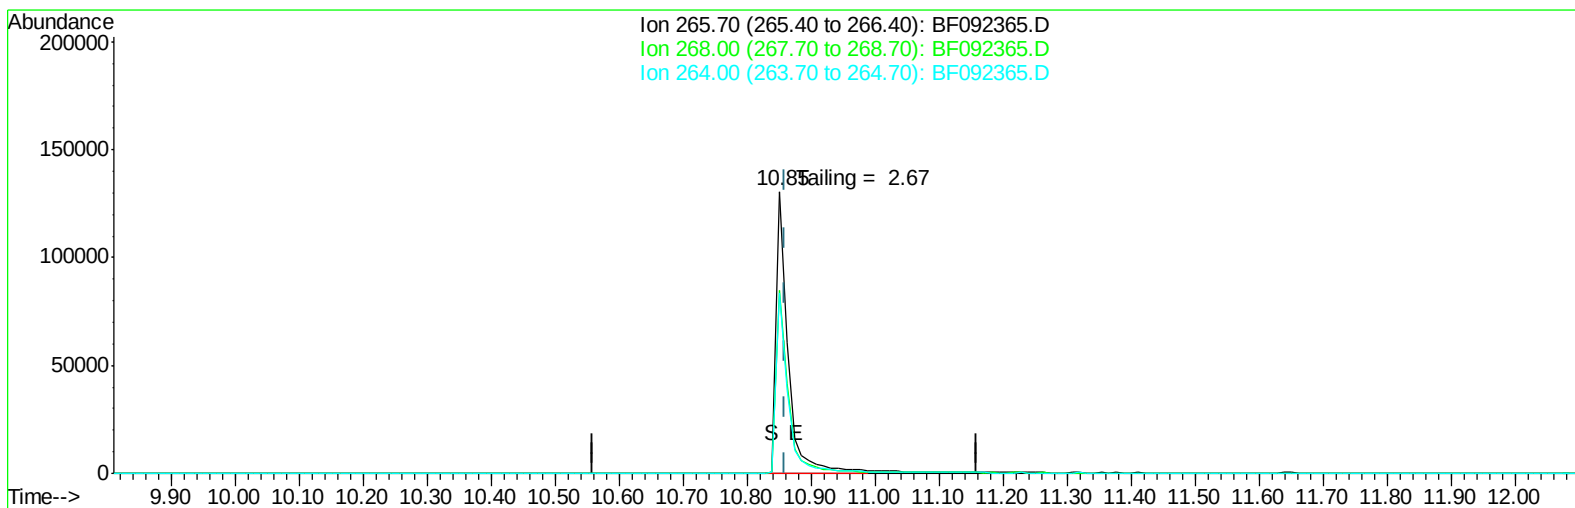

TIC: BF092365.D

(69) Pentachlorophenol (C)




10.851min (-0.009) 0.00ng

response 171335

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.01
264.00	62.90	63.98
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF012017\
Data File : BF092365.D
Acq On : 20 Jan 2017 10:51
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 07:27:44 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 23 01:12:17 2017
Response via : Initial Calibration

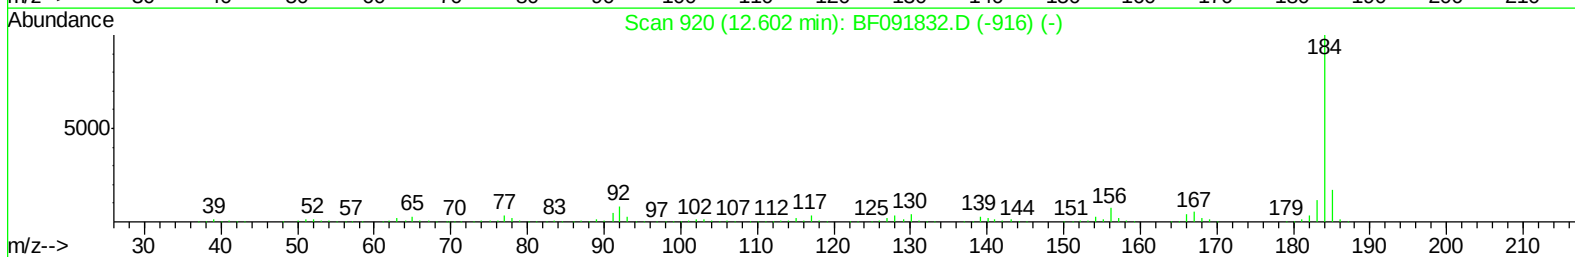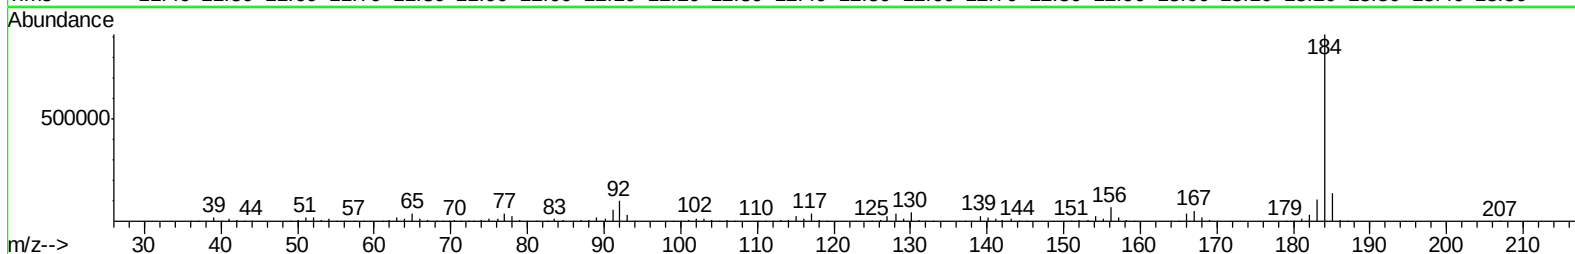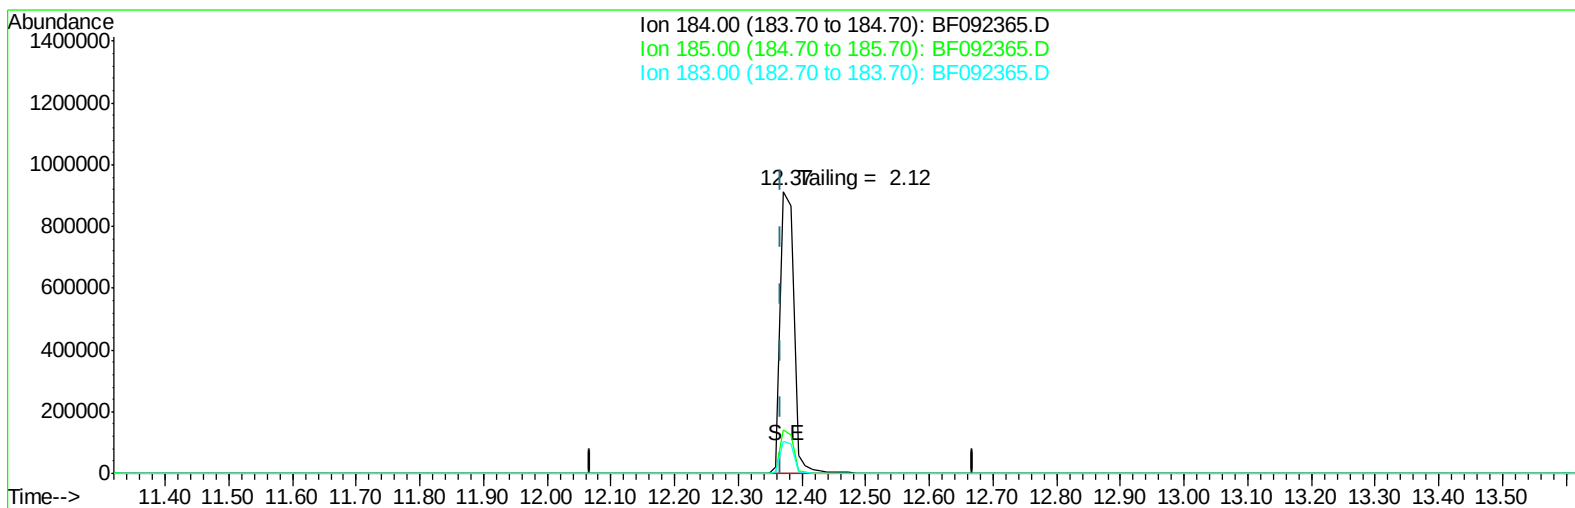

TIC: BF092365.D

(76) Benzidine

12.371min (+0.003) 0.00ng

response 1322863

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.28
183.00	11.50	11.48
0.00	0.00	0.00