


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012017\
 Data File : BF092390.D
 Acq On : 21 Jan 2017 00:30
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

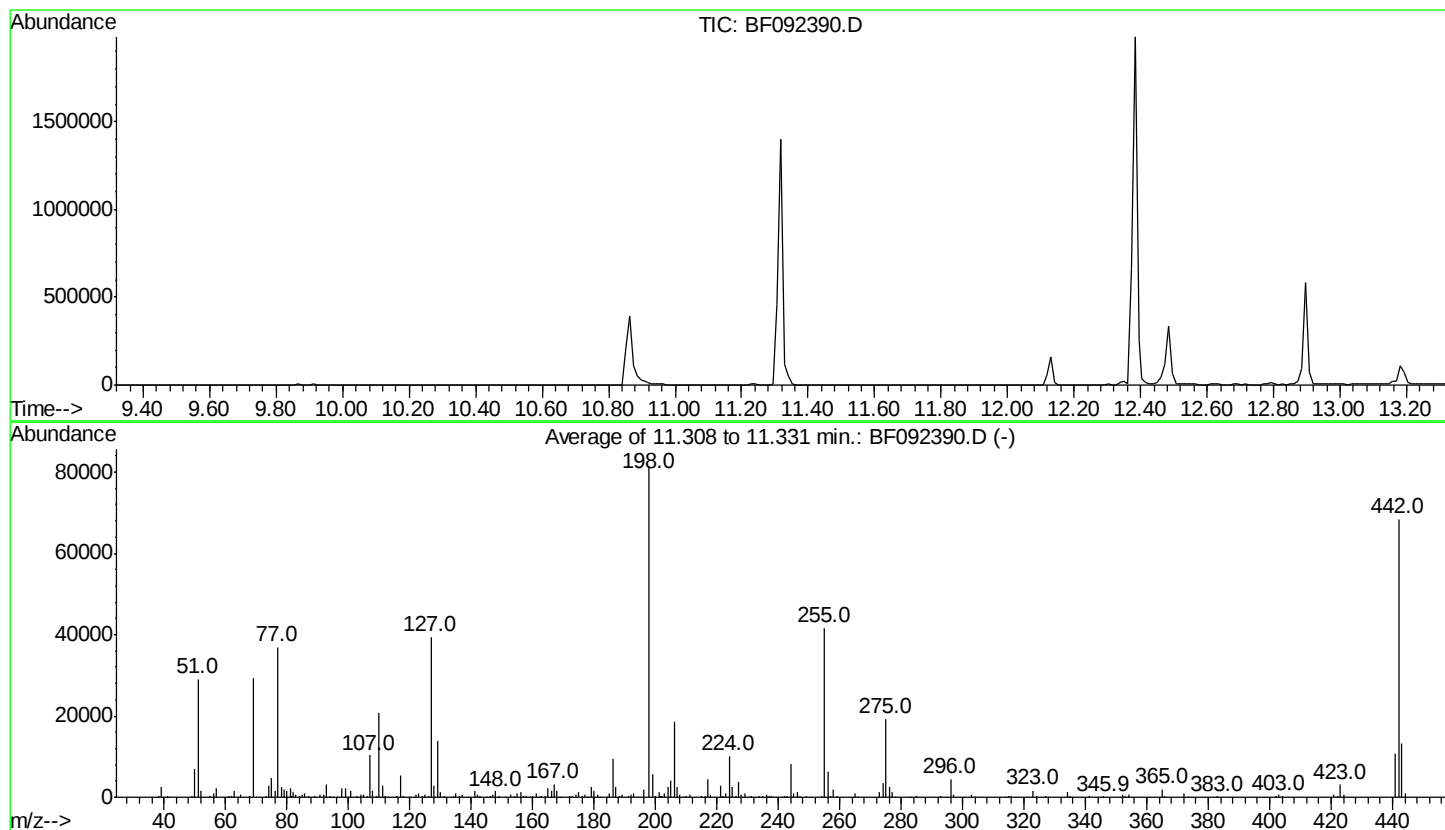

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	29099	PASS
68	69	0.00	2	1.6	470	PASS
69	198	0.00	100	36.1	29427	PASS
70	69	0.00	2	0.3	101	PASS
127	198	10	80	48.3	39430	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81587	PASS
199	198	5	9	6.9	5663	PASS
275	198	10	60	23.6	19279	PASS
365	198	1	100	2.5	2009	PASS
441	442	0.01	24	15.5	10630	PASS
442	198	50	100	83.9	68450	PASS
443	442	15	24	19.3	13233	PASS