
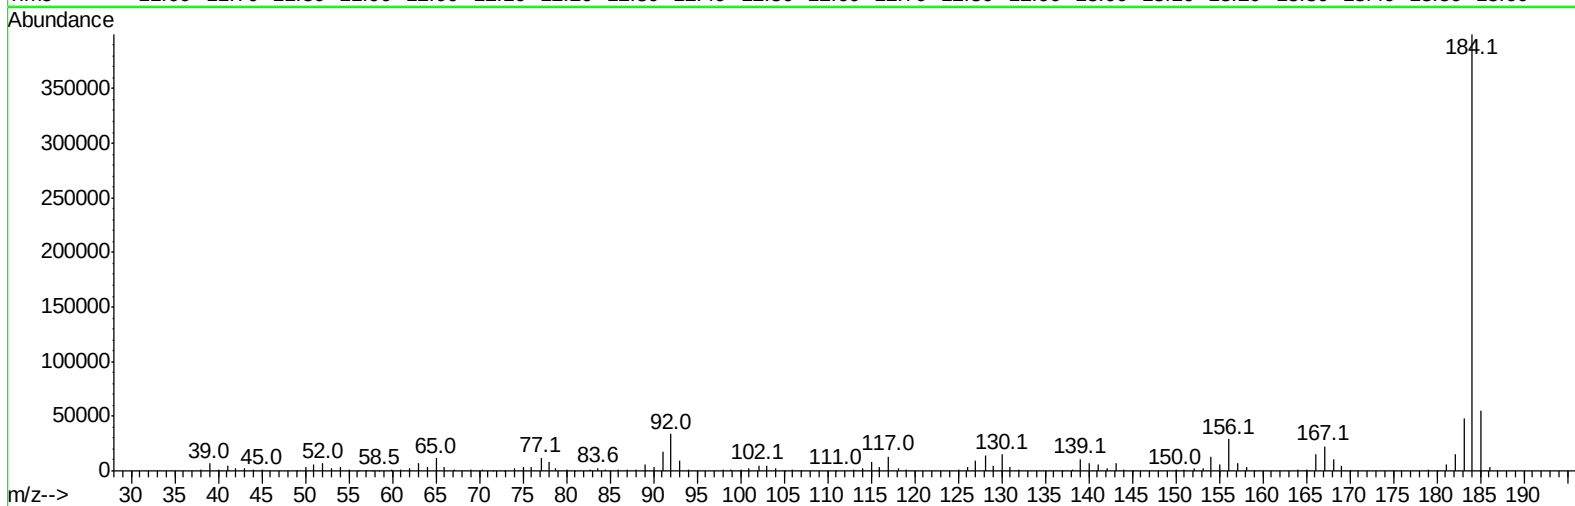


Data Path : U:\HPCHEM1\BNA F\DATA\BF012018\
Data File : BF102251.D
Acq On : 20 Jan 2018 8:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 04:47:27 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 13:31:35 2018
Response via : Initial Calibration

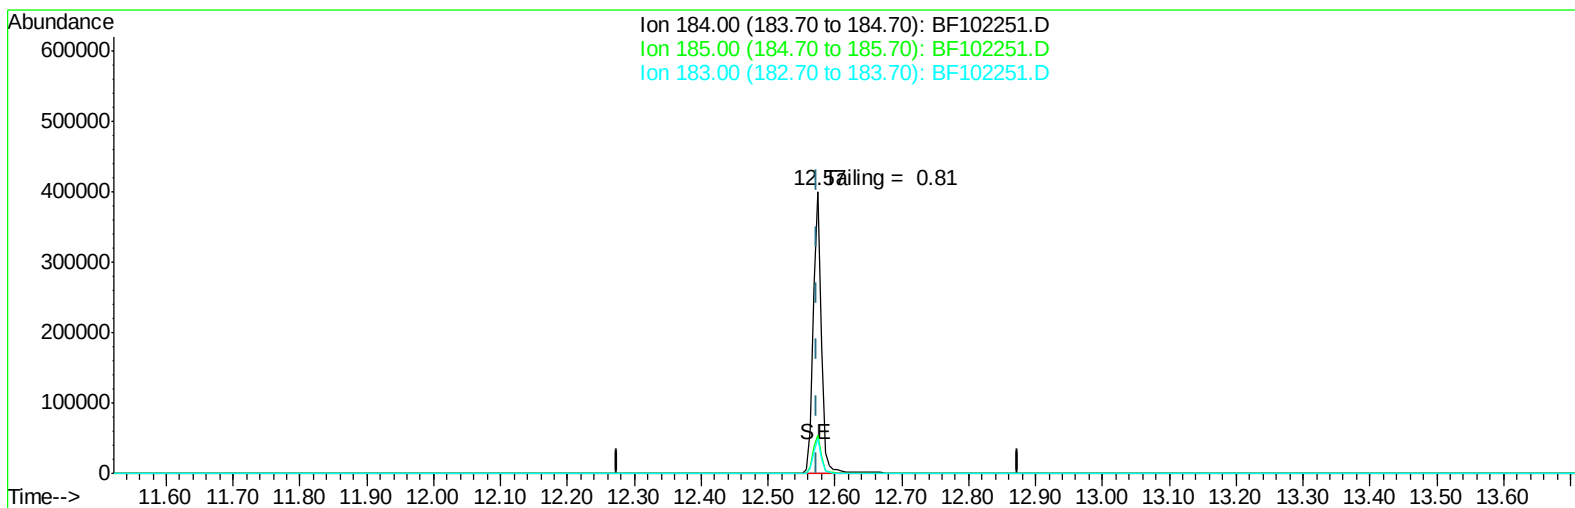

TIC: BF102251.D

(76) Benzidine




12.574min (+0.000) 0.00ng

response 347164

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.84
183.00	11.60	12.16
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF012018\
Data File : BF102251.D
Acq On : 20 Jan 2018 8:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 04:47:27 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 13:31:35 2018
Response via : Initial Calibration

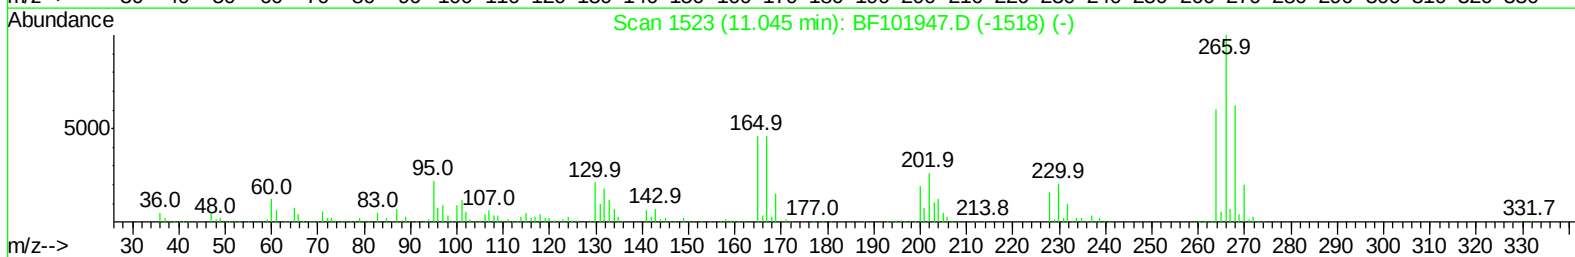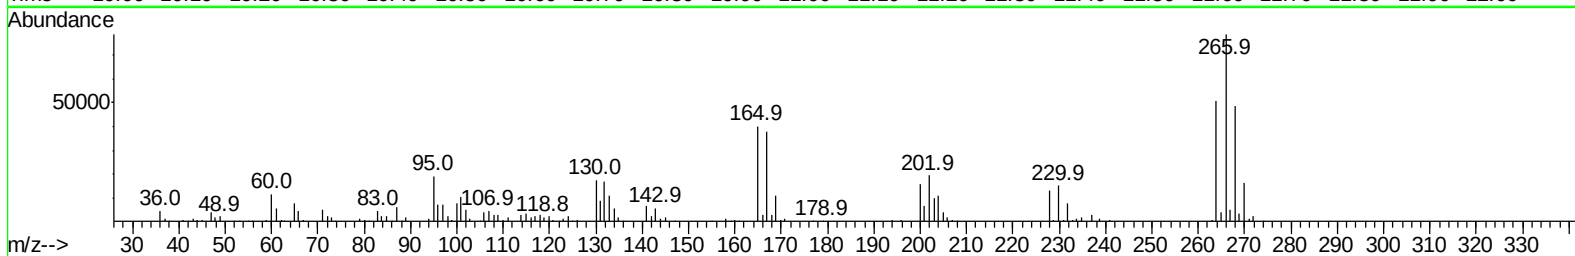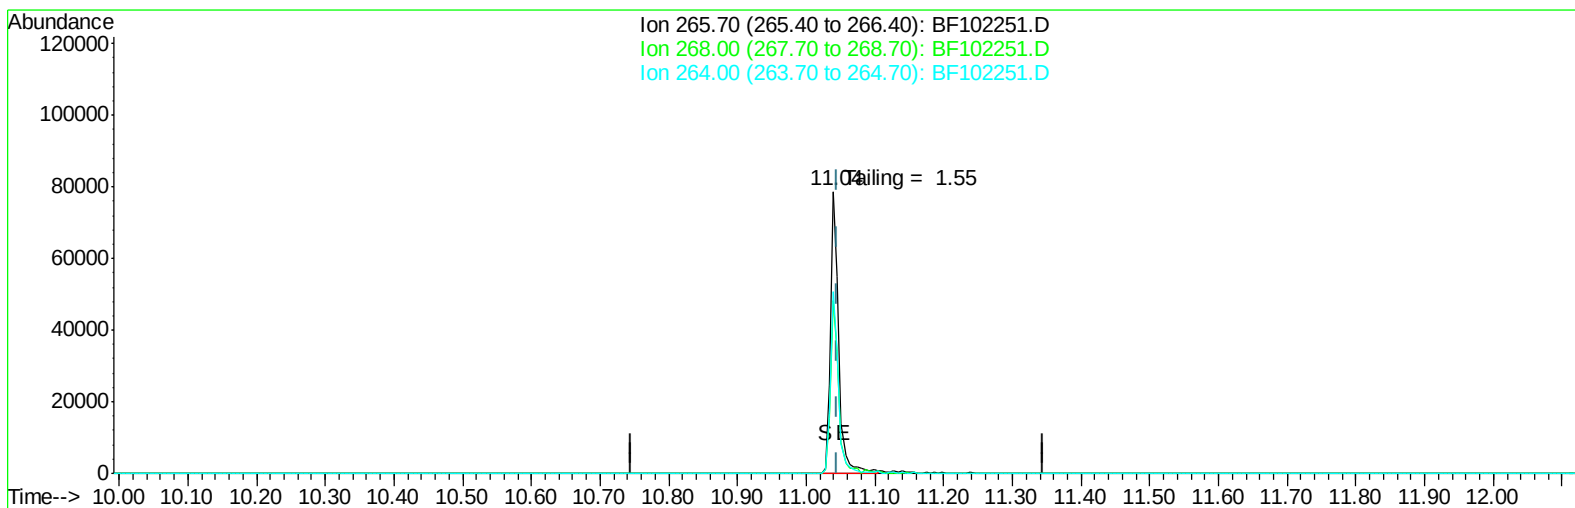

TIC: BF102251.D

(69) Pentachlorophenol (C)

11.039min (-0.006) 24599.67ng

response 67273

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.54
264.00	61.90	64.78
0.00	0.00	0.00