
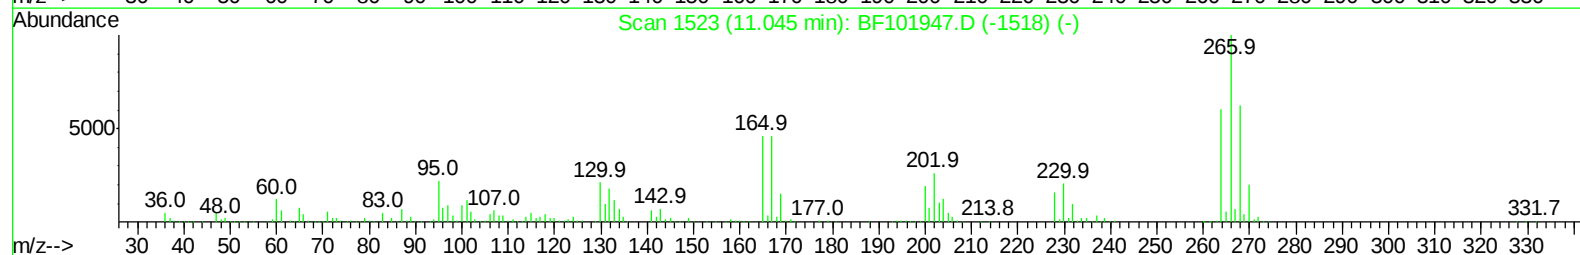
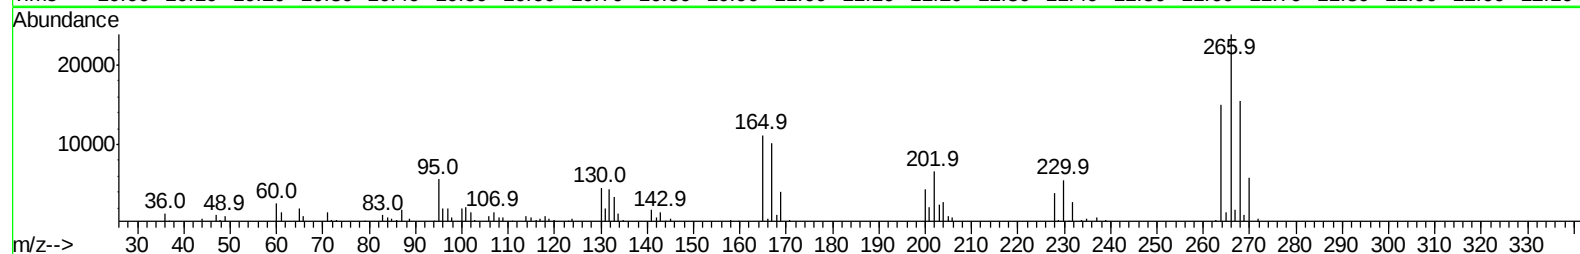


Data Path : U:\HPCHEM1\BNA F\DATA\BF012018\
Data File : BF102278.D
Acq On : 20 Jan 2018 22:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 04:51:11 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 13:31:35 2018
Response via : Initial Calibration

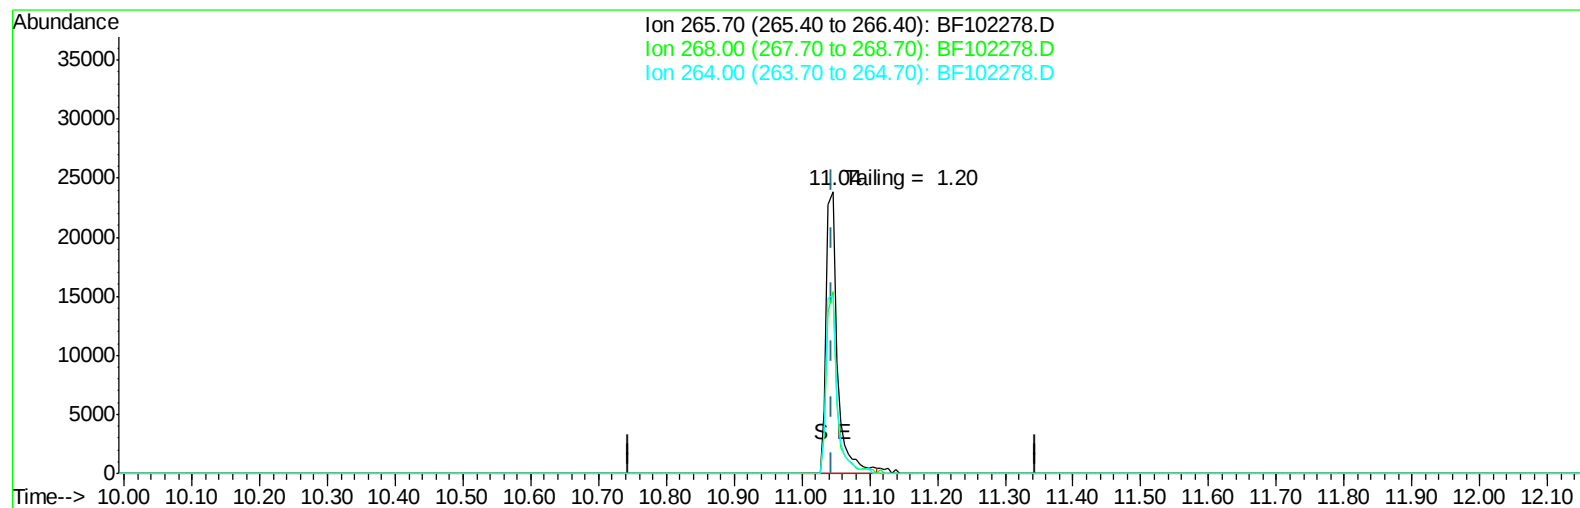

TIC: BF102278.D

(69) Pentachlorophenol (C)




11.045min (+0.000) 21504.62ng

response 26910

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.60
264.00	61.90	63.02
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF012018\
Data File : BF102278.D
Acq On : 20 Jan 2018 22:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 04:51:11 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 13:31:35 2018
Response via : Initial Calibration

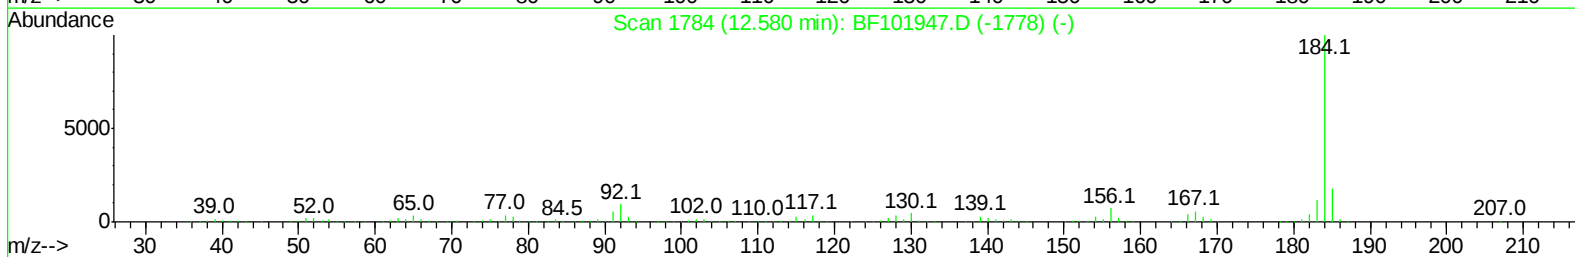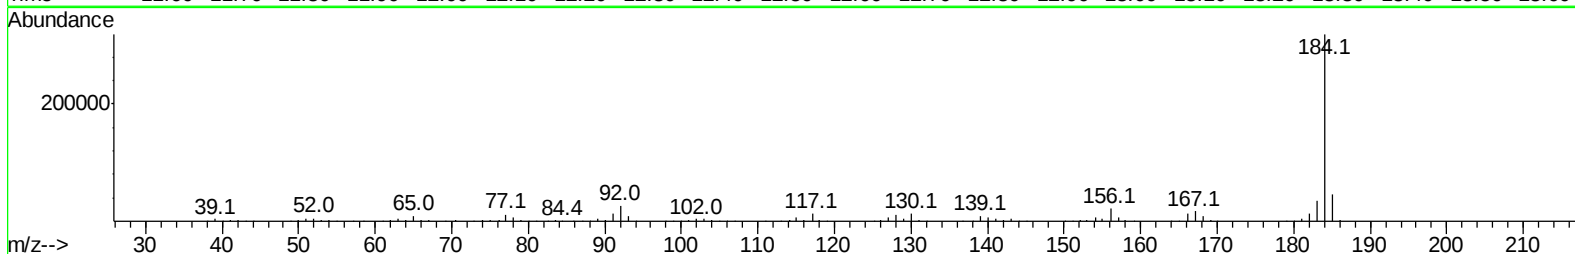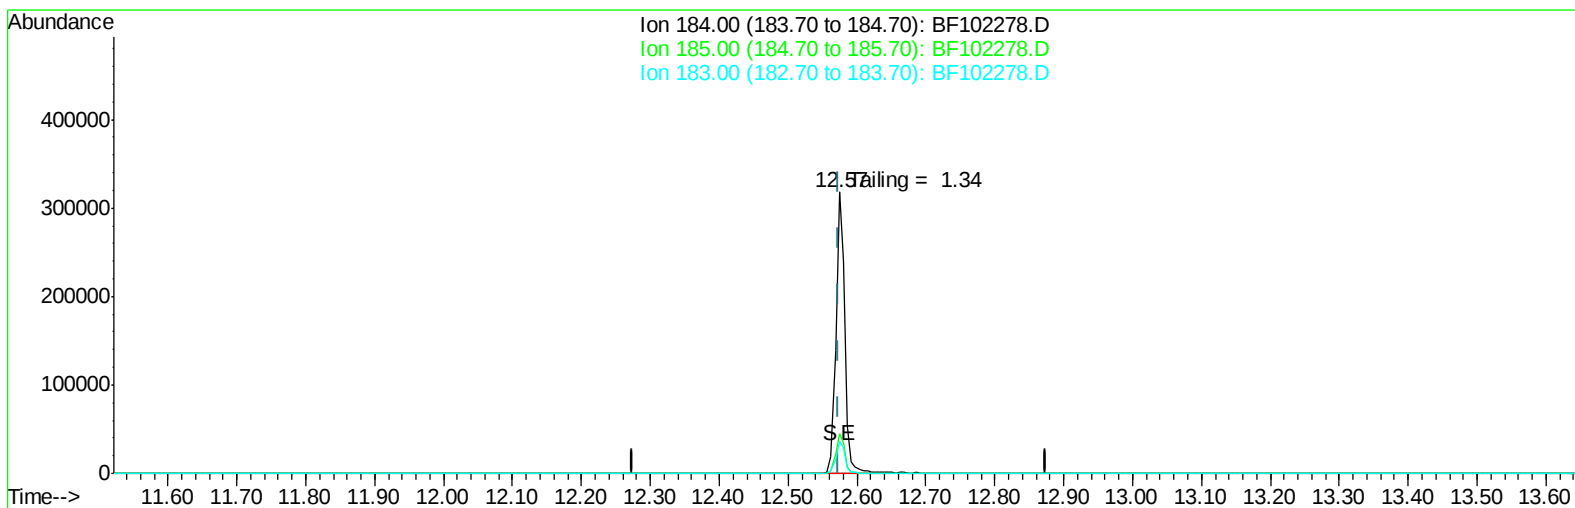

TIC: BF102278.D

(76) Benzidine

12.574min (0.000) 0.00ng

response 285990

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.30
183.00	11.60	11.36
0.00	0.00	0.00