

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012018\
 Data File : BF102283.D
 Acq On : 21 Jan 2018 1:17
 Operator : SJ/JU
 Sample : J1189-04DL 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 22C-2DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.387	49	51	58	rVB	33597	49325	1.91%	0.437%
2	4.893	474	477	487	rBV	64587	67659	2.63%	0.599%
3	5.169	521	524	528	rVB	27303	25832	1.00%	0.229%
4	5.281	538	543	546	rBV	123909	132492	5.14%	1.174%
5	5.316	546	549	559	rVB	418933	402491	15.62%	3.566%
6	5.546	584	588	592	rBV	115809	101650	3.95%	0.901%
7	5.651	602	606	612	rBV2	33760	40304	1.56%	0.357%
8	6.351	721	725	732	rBV	463603	441750	17.15%	3.914%
9	6.481	744	747	751	rBV	472502	421630	16.36%	3.736%
10	6.540	754	757	763	rVB2	26210	26001	1.01%	0.230%
11	6.716	784	787	791	rBV	943658	771828	29.96%	6.839%
12	6.869	810	813	817	rBV	397323	328147	12.74%	2.908%
13	7.281	880	883	887	rBV	268315	229245	8.90%	2.031%
14	7.998	1001	1005	1009	rBV	1177918	1014049	39.36%	8.985%
15	9.075	1183	1188	1199	rBV	589132	482718	18.74%	4.277%
16	9.469	1252	1255	1264	rVB	44457	45601	1.77%	0.404%
17	9.598	1273	1277	1280	rVB	42163	35288	1.37%	0.313%
18	9.751	1300	1303	1314	rBV	1081088	963987	37.42%	8.541%
19	10.539	1433	1437	1445	rBV	198610	174811	6.78%	1.549%
20	10.657	1453	1457	1466	rVB2	23585	29375	1.14%	0.260%
21	10.786	1476	1479	1484	rBV	36982	29976	1.16%	0.266%
22	11.233	1552	1555	1559	rBV	860610	773200	30.01%	6.851%
23	11.798	1648	1651	1655	rBV	1104296	907097	35.21%	8.037%
24	12.816	1820	1824	1828	rBV	357400	303287	11.77%	2.687%
25	13.069	1860	1867	1871	rBV4	18842	31584	1.23%	0.280%
26	13.298	1903	1906	1909	rBV	326805	276080	10.72%	2.446%
27	13.857	1997	2001	2007	rBV2	2210709	2576469	100.00%	22.829%
28	15.292	2240	2245	2253	rBV	498367	604138	23.45%	5.353%


Sum of corrected areas: 11286014

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012018\
Data File : BF102283.D
Acq On : 21 Jan 2018 1:17
Operator : SJ/JU
Sample : J1189-04DL 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
22C-2DL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

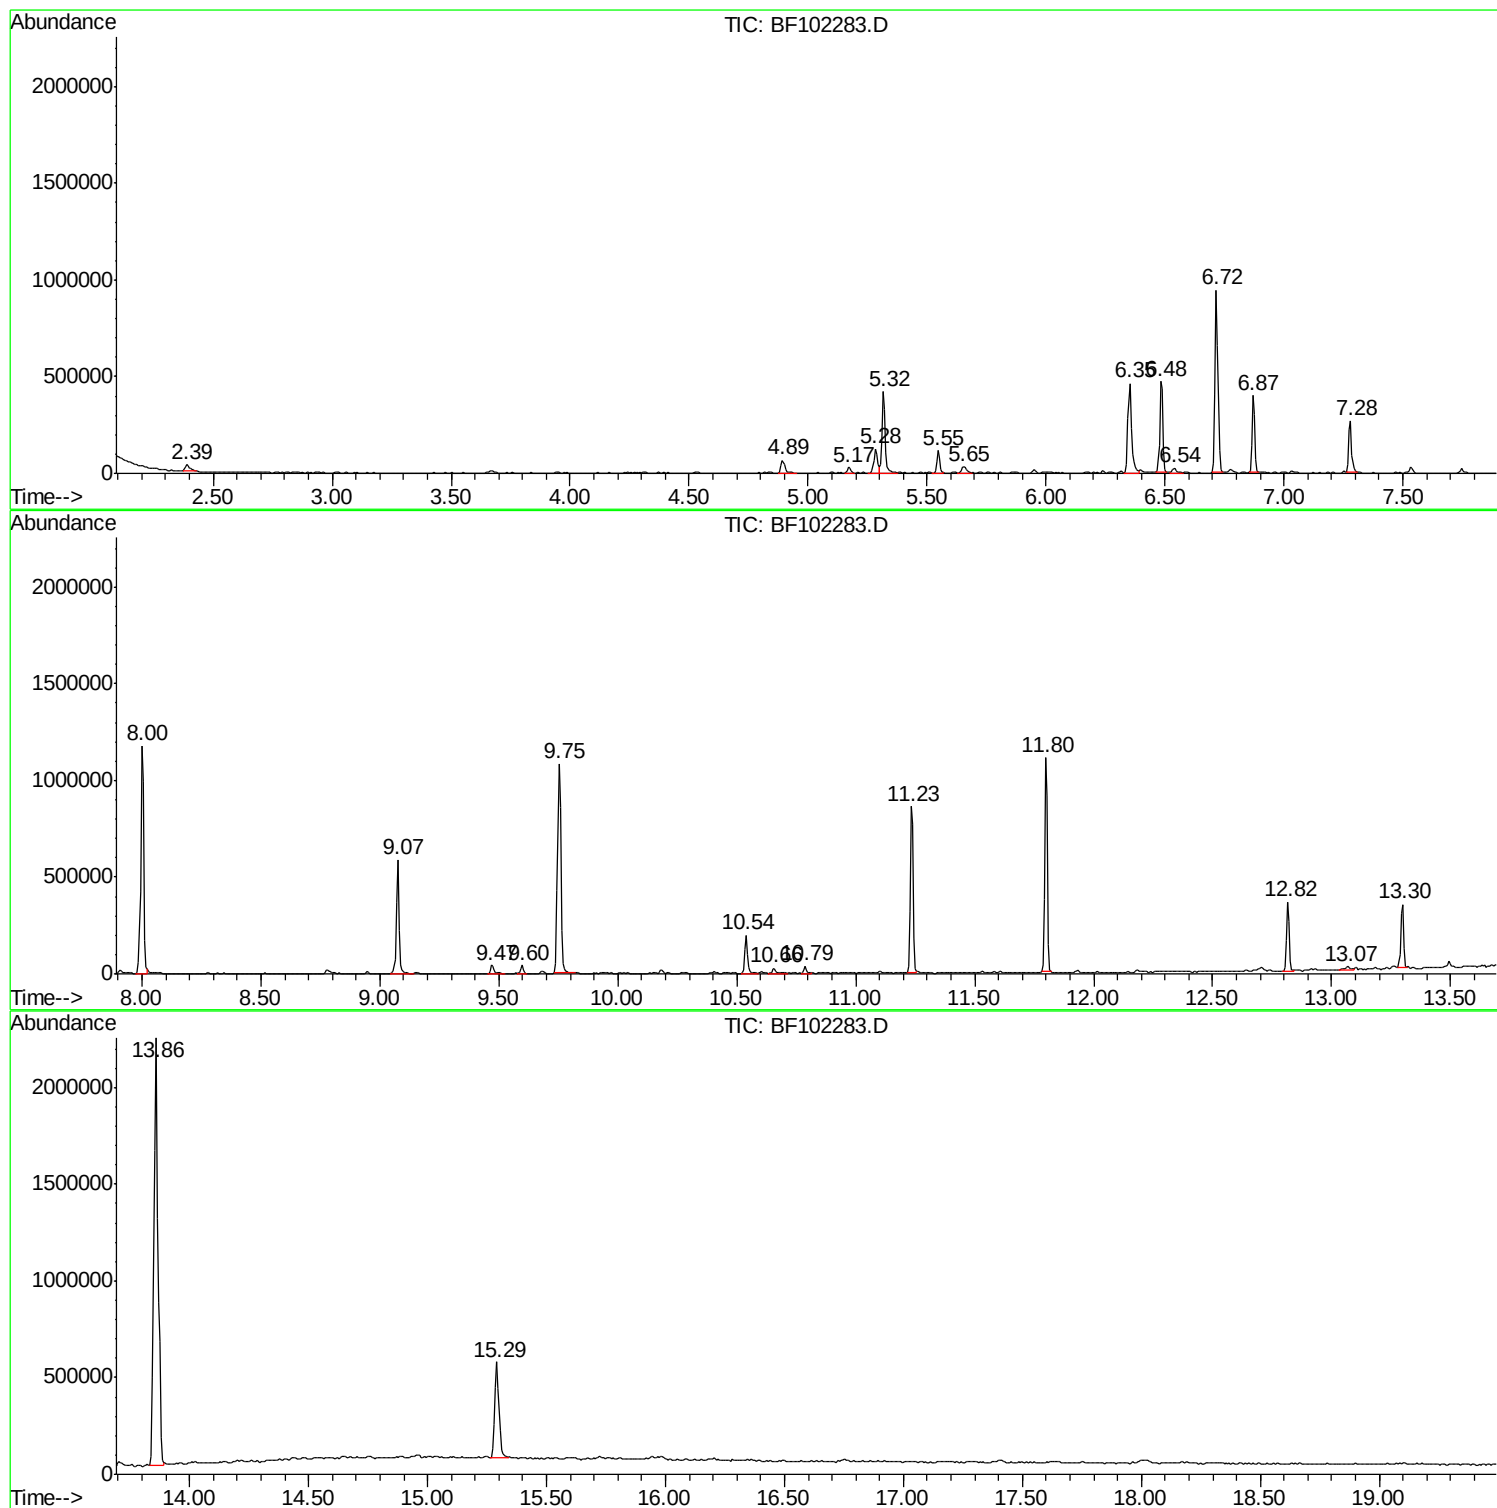

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012018\
Data File : BF102283.D
Acq On : 21 Jan 2018 1:17
Operator : SJ/JU
Sample : J1189-04DL 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
22C-2DL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.48 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	10.93 ng	421630	1,4-Dichlorobenzene-d4	6.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

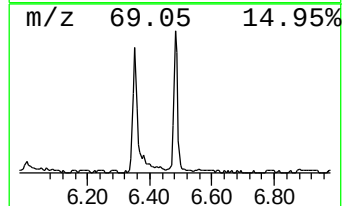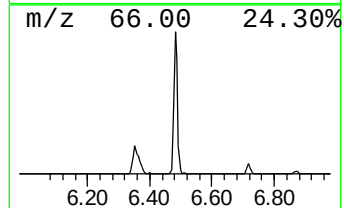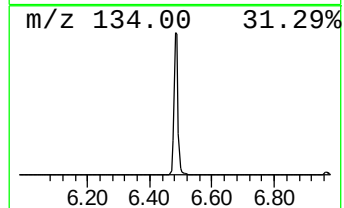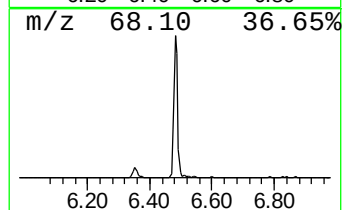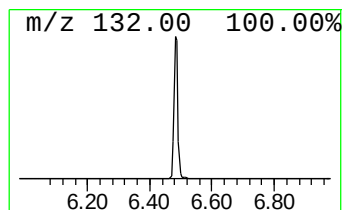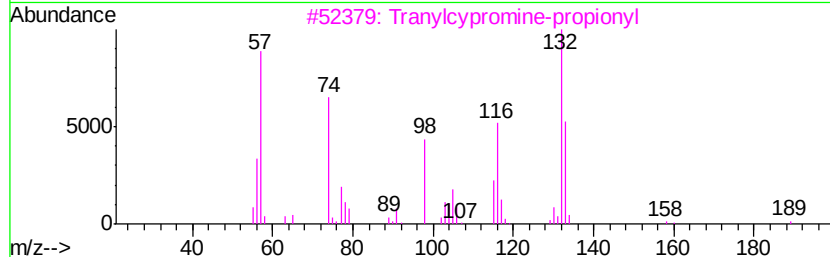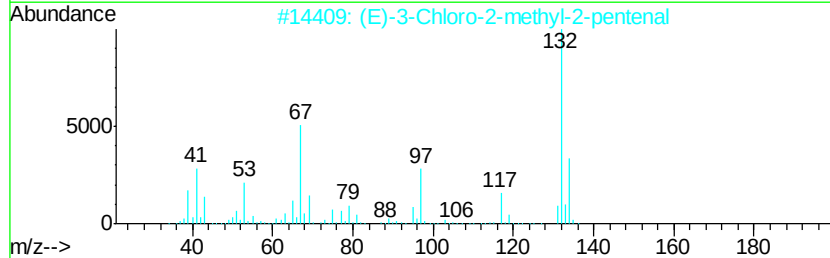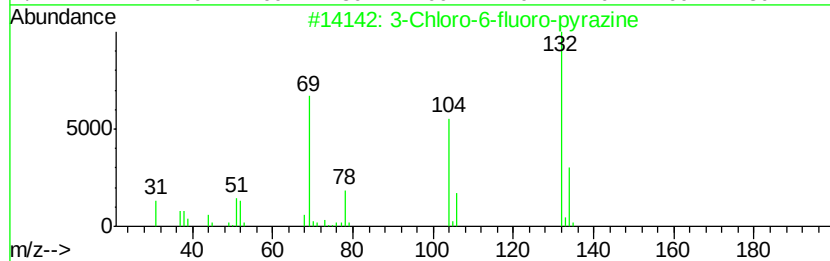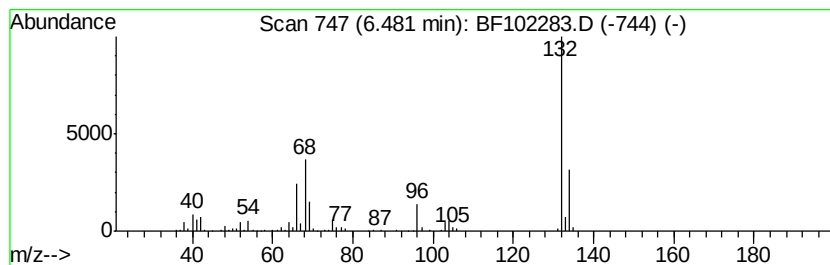

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012018\
Data File : BF102283.D
Acq On : 21 Jan 2018 1:17
Operator : SJ/JU
Sample : J1189-04DL 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
22C-2DL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.48	6.48	10.9	ng	421630	1	6.72	771828	20.0