


Data Path : Z:\HPCHEM1\BNA F\Data\BF012018\  
 Data File : BF102251.D  
 Acq On : 20 Jan 2018 8:28  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF010918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jan 19 13:31:35 2018

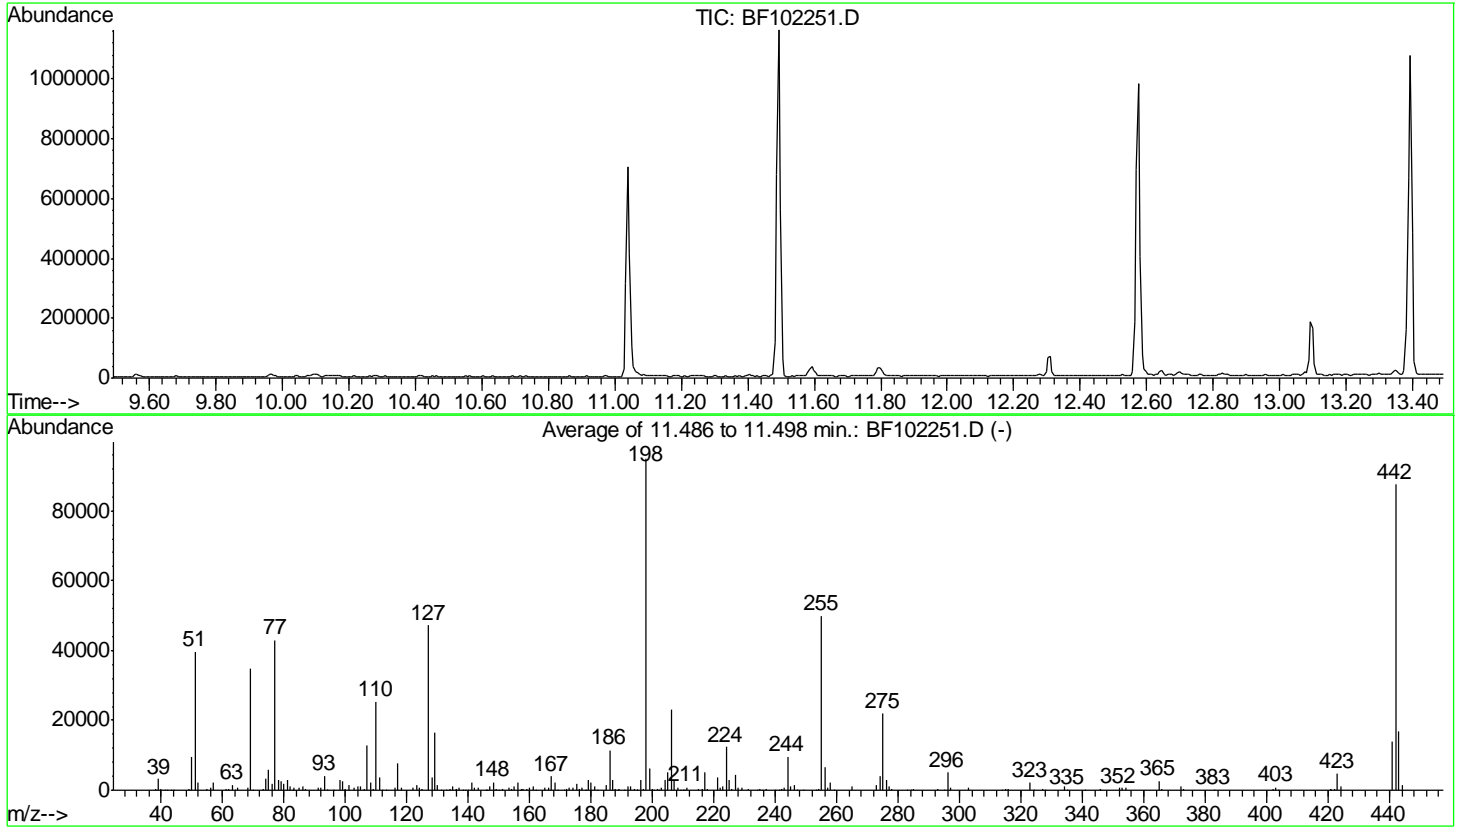

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	39752	PASS
68	69	0.00	2	1.6	574	PASS
69	198	0.00	100	36.7	34805	PASS
70	69	0.00	2	0.3	121	PASS
127	198	10	80	49.8	47234	PASS
197	198	0.00	2	0.3	238	PASS
198	198	100	100	100.0	94914	PASS
199	198	5	9	6.5	6137	PASS
275	198	10	60	23.0	21839	PASS
365	198	1	100	2.8	2685	PASS
441	443	0.01	100	82.2	13875	PASS
442	198	50	100	92.2	87504	PASS
443	442	15	24	19.3	16876	PASS