
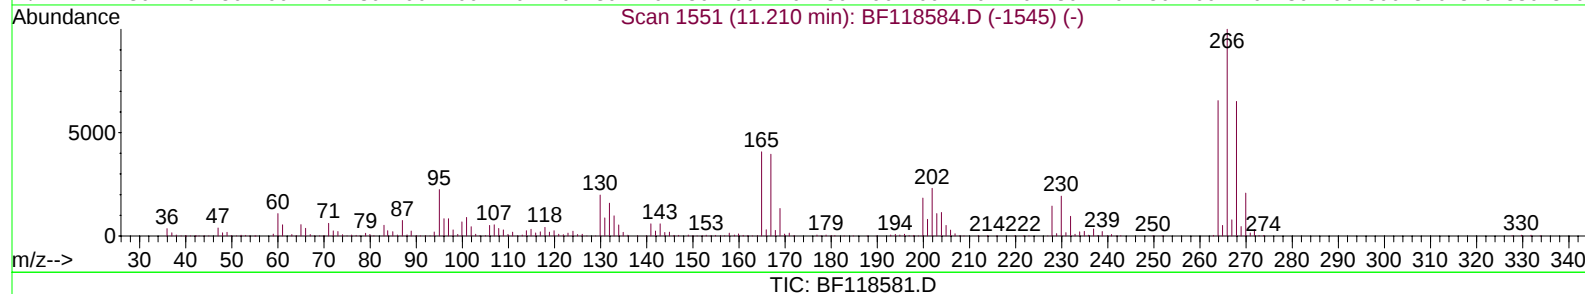
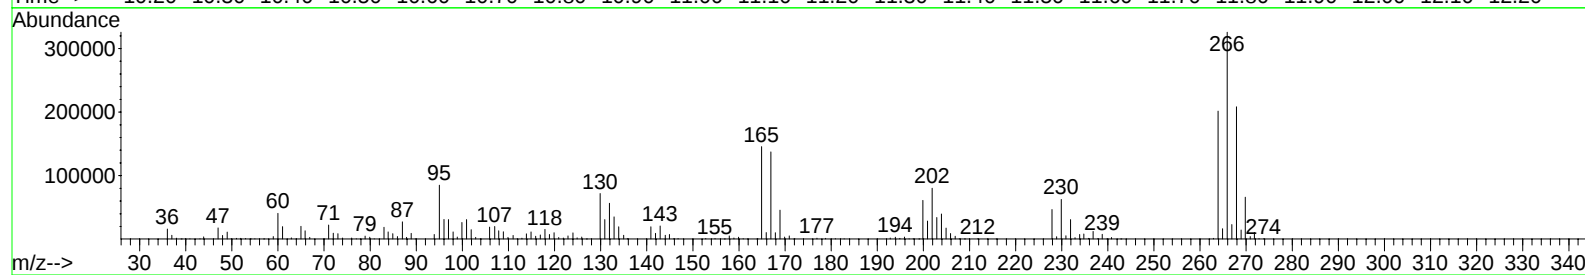


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012020\
Data File : BF118581.D
Acq On : 20 Jan 2020 10:12
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 18:18:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 20 14:45:03 2020
Response via : Initial Calibration

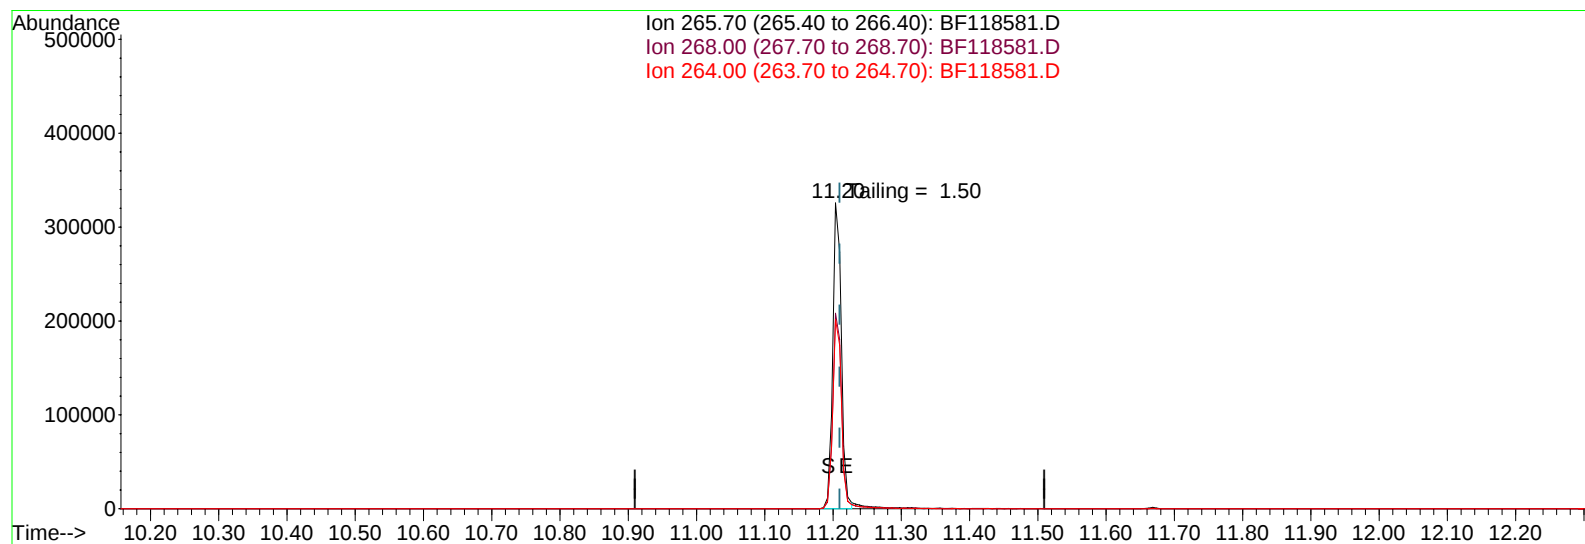

(70) Pentachlorophenol (C)




11.204min (-0.006) 25371.78ng

response 290254

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	63.94
264.00	65.50	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012020\
Data File : BF118581.D
Acq On : 20 Jan 2020 10:12
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 18:18:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 20 14:45:03 2020
Response via : Initial Calibration

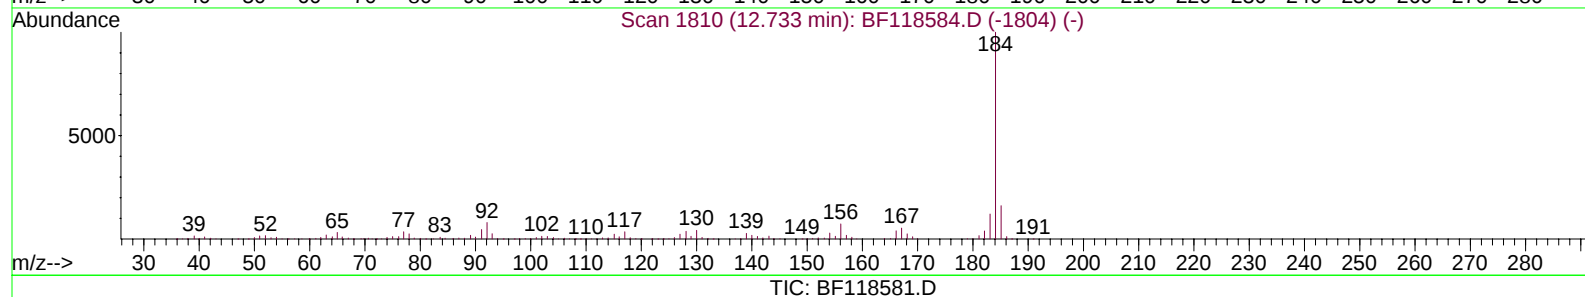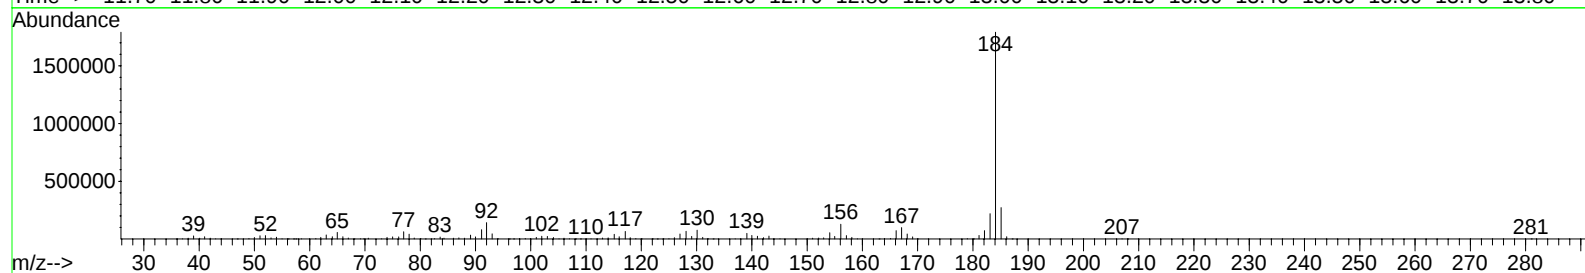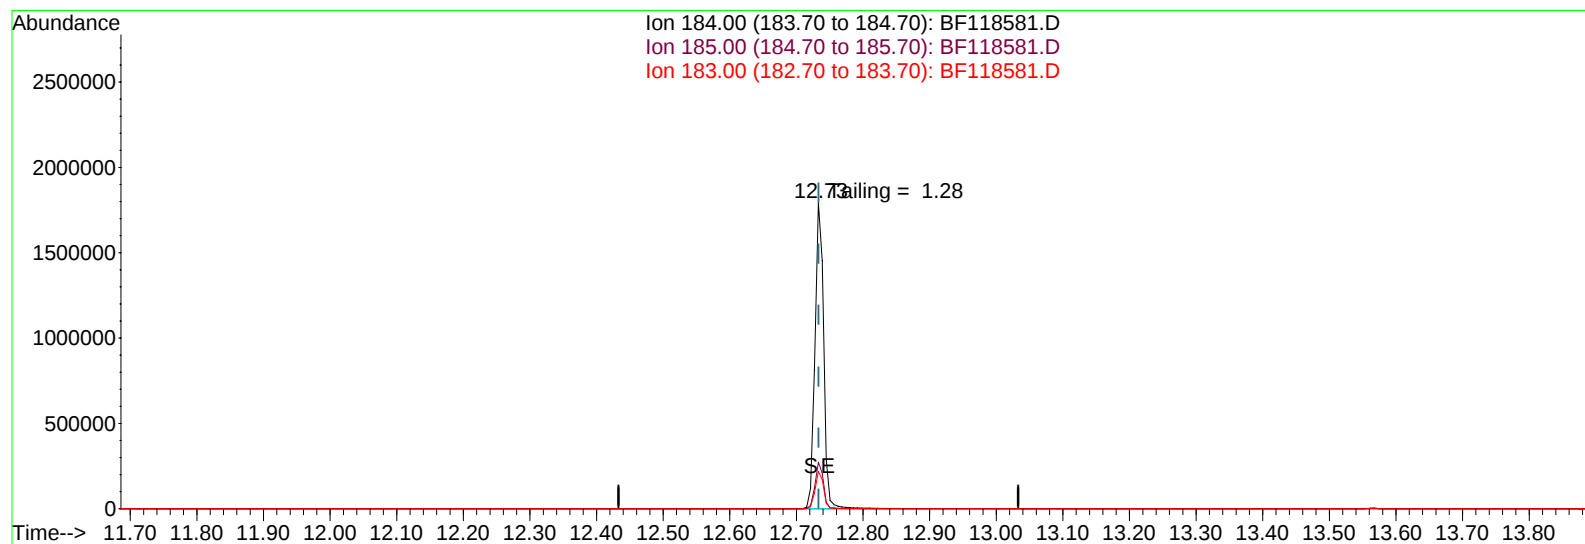

(77) Benzidine

12.733min (-0.000) 0.00ng

response 1635964

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	15.23
183.00	12.00	12.22
0.00	0.00	0.00