
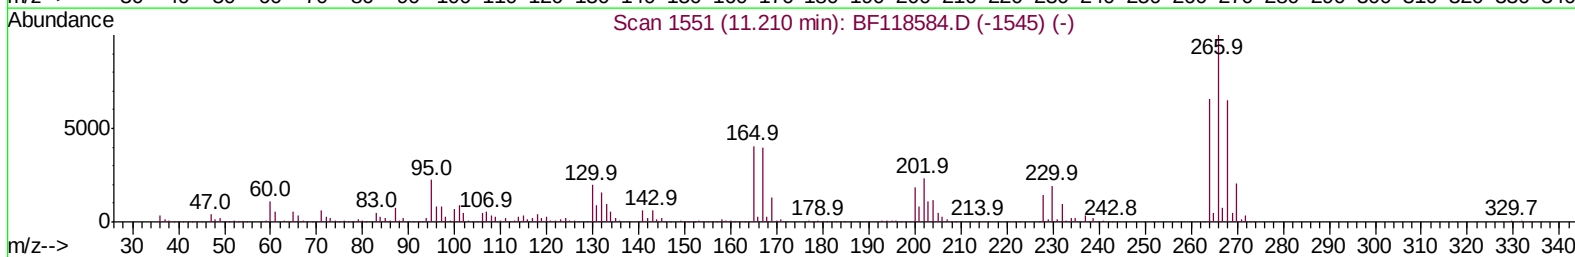
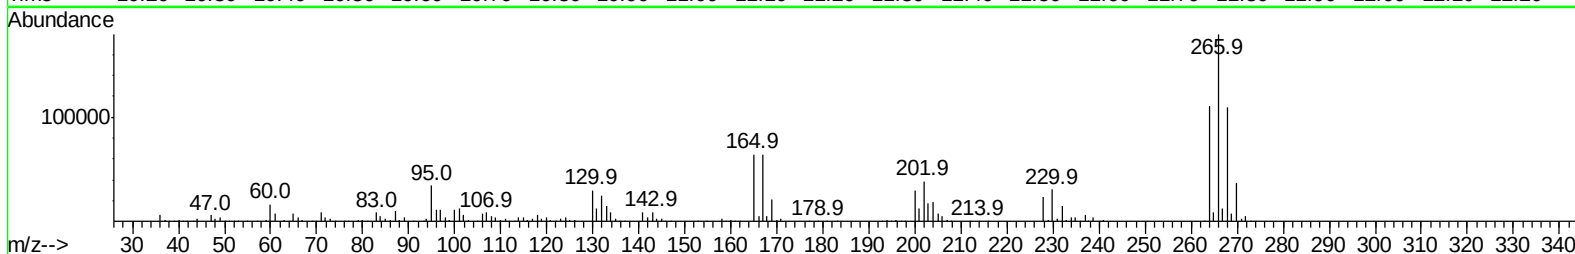


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF012020\  
Data File : BF118617.D  
Acq On : 21 Jan 2020 4:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 08:38:09 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 20 14:45:03 2020  
Response via : Initial Calibration

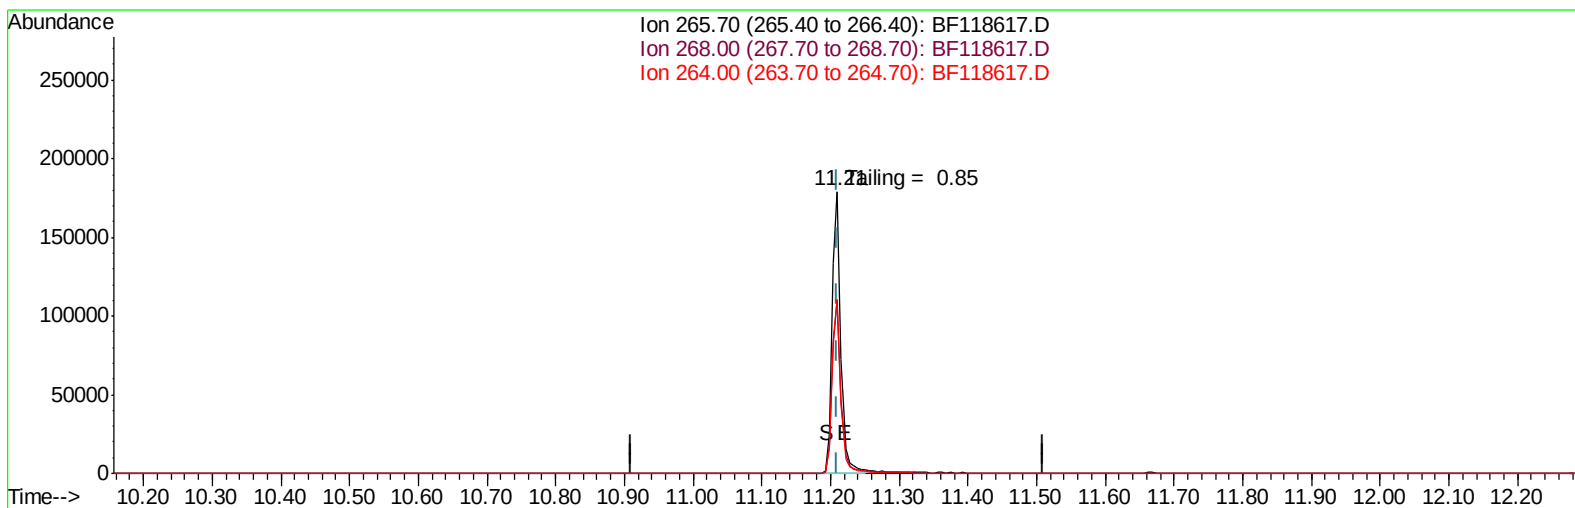

TIC: BF118617.D

(70) Pentachlorophenol (C)




11.210min (+0.000) 181440.42ng

response 161081

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.10 | 61.20 |
| 264.00 | 65.50 | 61.78 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF012020\  
Data File : BF118617.D  
Acq On : 21 Jan 2020 4:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 08:38:09 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 20 14:45:03 2020  
Response via : Initial Calibration

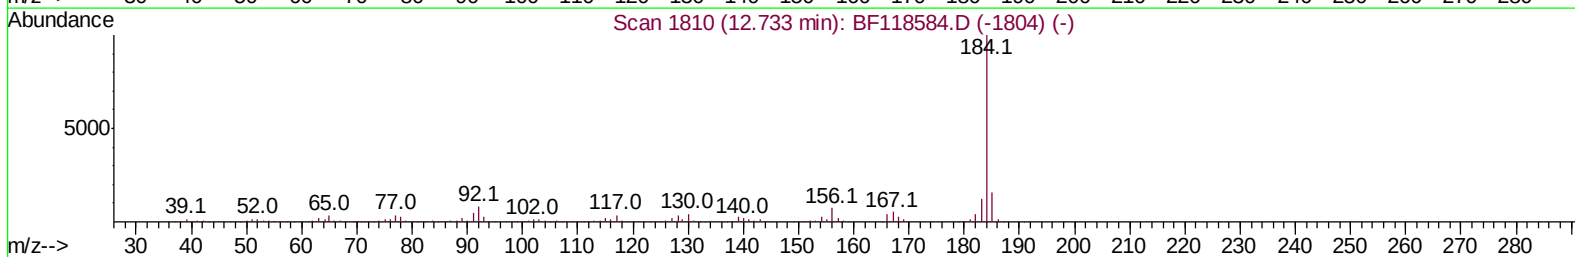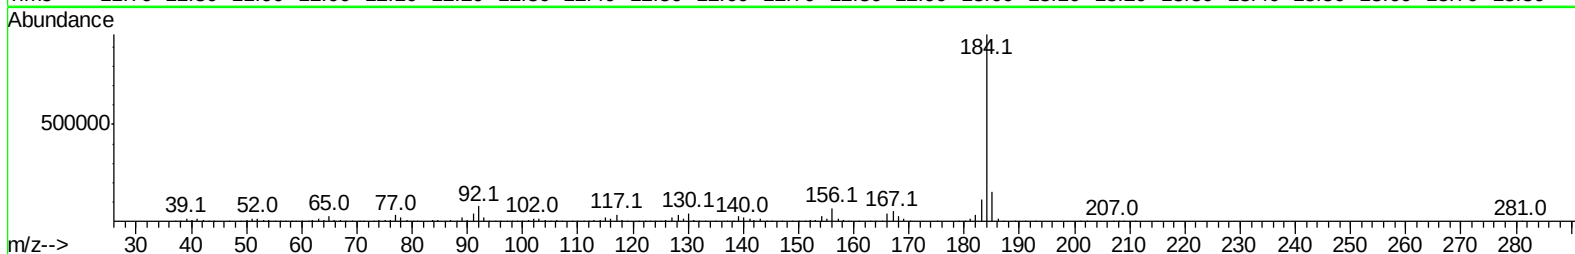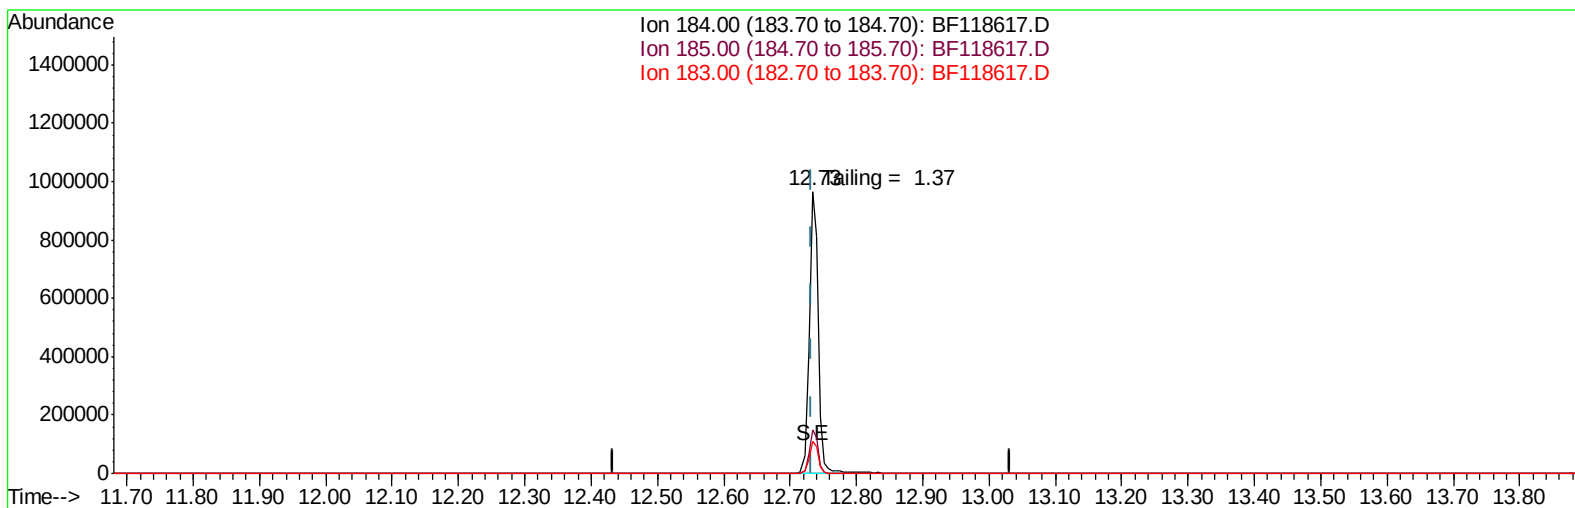

TIC: BF118617.D

(77) Benzidine

12.733min (+0.000) 94065.97ng

response 909839

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.10 | 15.61 |
| 183.00 | 12.00 | 11.60 |
| 0.00   | 0.00  | 0.00  |