

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF012020\
 Data File : BF118595.D
 Acq On : 20 Jan 2020 17:07
 Operator : CG/JU
 Sample : L1154-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B3-15-20

Quant Time: Jan 21 01:59:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 20 14:45:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	462095	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	1686385	20.00	ng	0.00
39) Acenaphthene-d10	9.92	164	969504	20.00	ng	-0.01
64) Phenanthrene-d10	11.40	188	1770612	20.00	ng	0.00
76) Chrysene-d12	14.04	240	1152666	20.00	ng	0.00
87) Perylene-d12	15.51	264	1077401	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	2610667	104.93	ng	0.00
7) Phenol-d6	6.50	99	3620526	111.96	ng	0.00
23) Nitrobenzene-d5	7.44	82	2281239	75.66	ng	0.00
42) 2,4,6-Tribromophenol	10.70	330	1277678	113.94	ng	0.00
45) 2-Fluorobiphenyl	9.24	172	4142744	70.23	ng	0.00
79) Terphenyl-d14	12.99	244	4694440	88.83	ng	0.00
Target Compounds						
10) Phenol	6.52	94	148224	4.022	ng	97
50) Dimethylphthalate	9.63	163	381843	6.045	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF012020\
Data File : BF118595.D
Acq On : 20 Jan 2020 17:07
Operator : CG/JU
Sample : L1154-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B3-15-20

Quant Time: Jan 21 01:59:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 20 14:45:03 2020
Response via : Initial Calibration

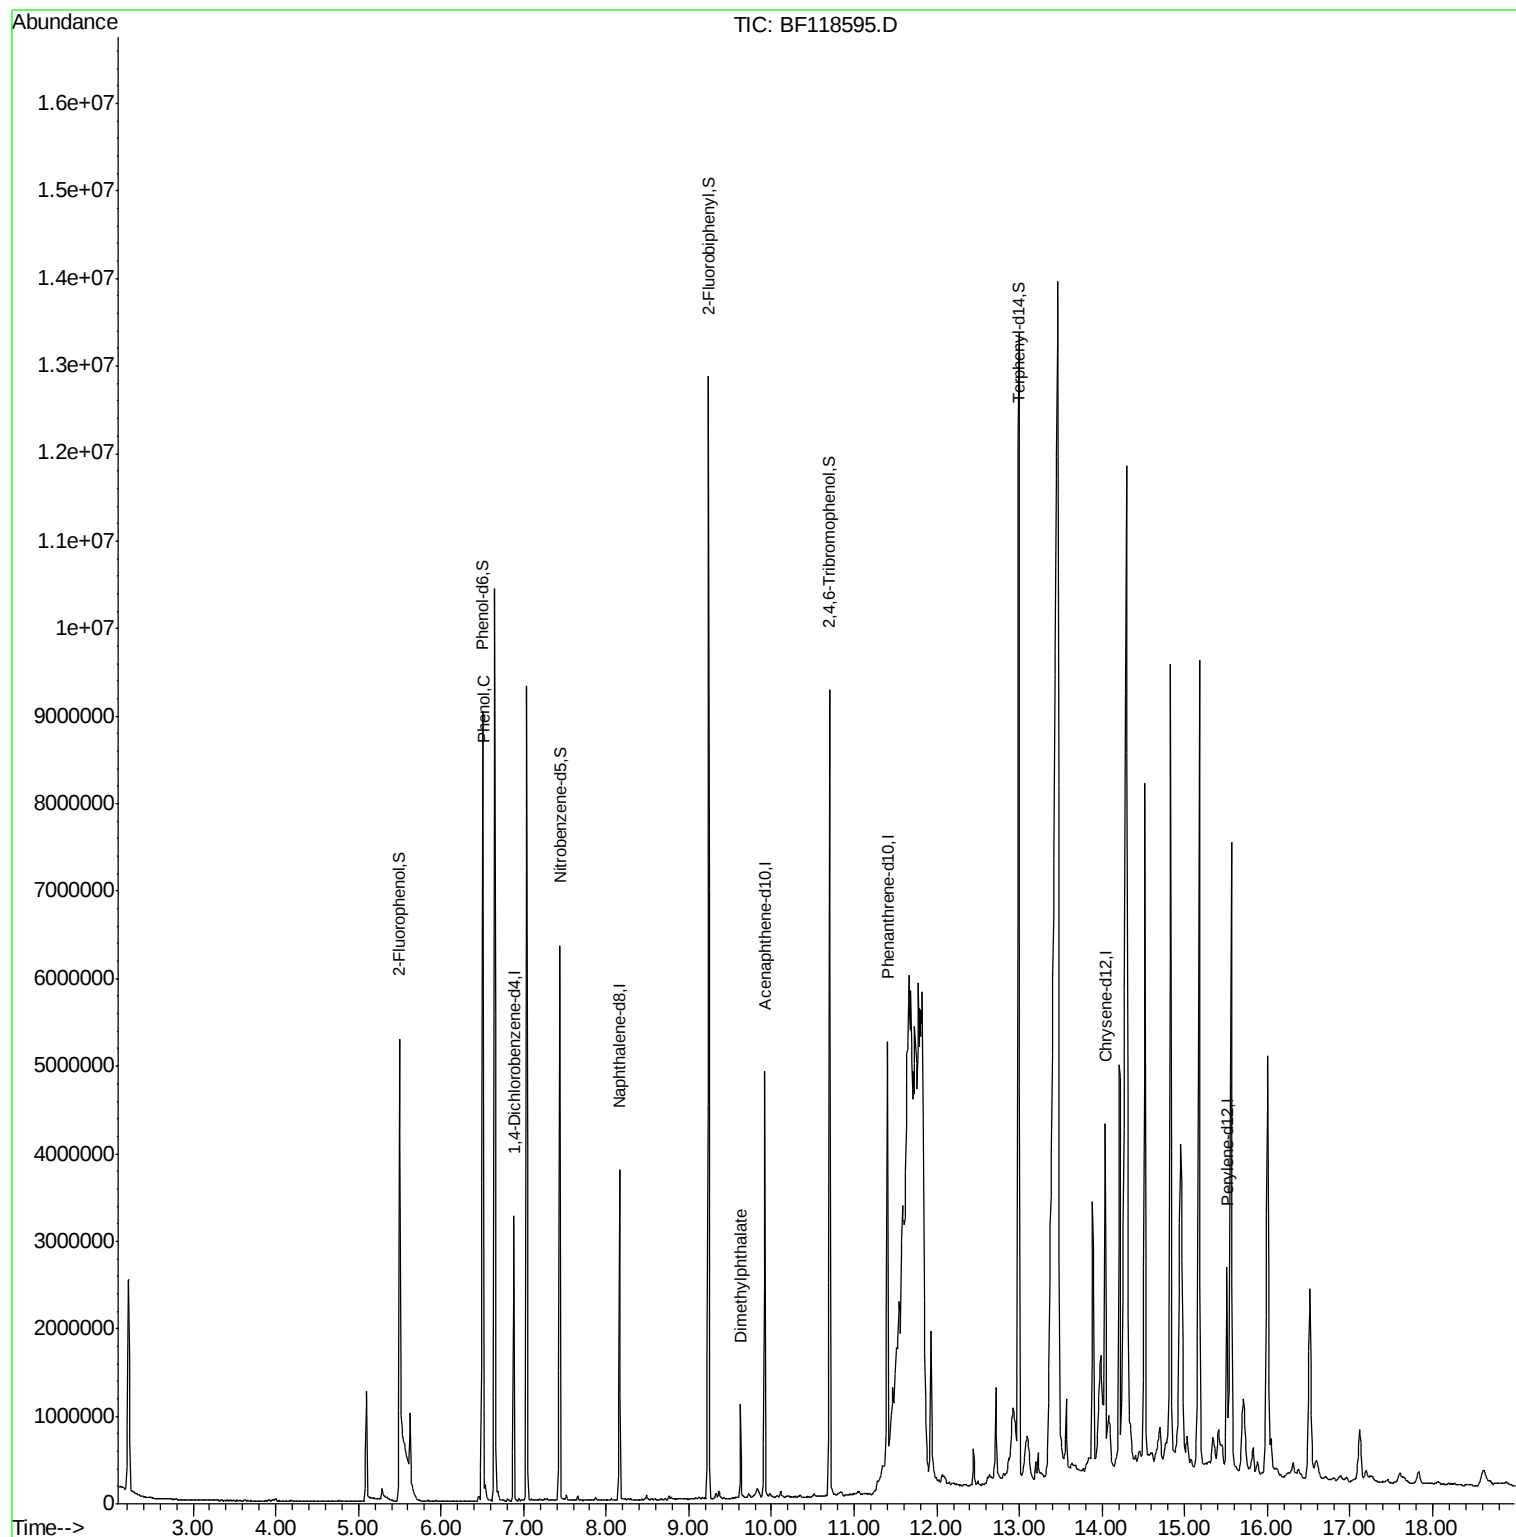




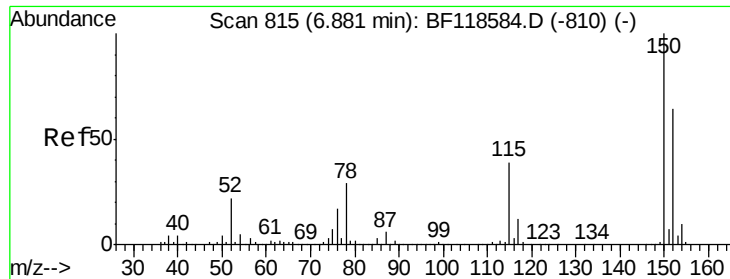


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.88 min Scan# 815
Delta R.T. 0.00 min
Lab File: BF118595.D
Acq: 20 Jan 2020 17:07

Instrument :
BNA_F
ClientSampleId :
B3-15-20




Tot Ion:152 Resp: 462095
Ion Ratio Lower Upper
152 100
150 155.6 125.6 188.4
115 58.2 48.4 72.6

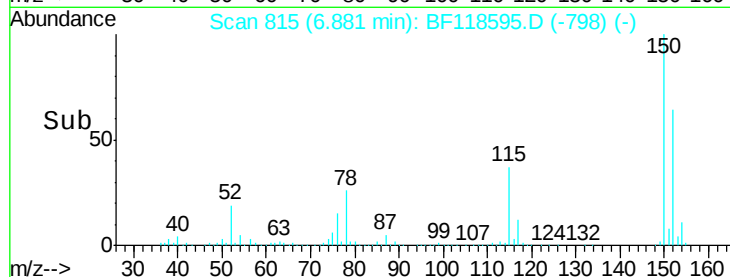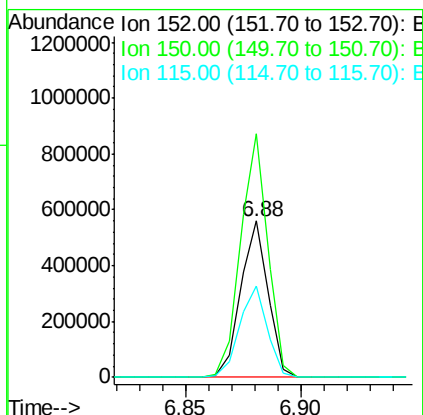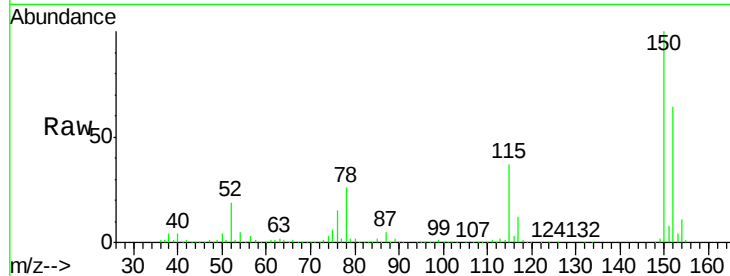

#5

2-Fluorophenol
Concen: 104.928 ng
RT: 5.50 min Scan# 580
Delta R.T. 0.00 min
Lab File: BF118595.D
Acq: 20 Jan 2020 17:07

Tgt Ion:112 Resp: 2610667
Ion Ratio Lower Upper
112 100
64 60.1 46.6 70.0
63 31.8 25.1 37.7

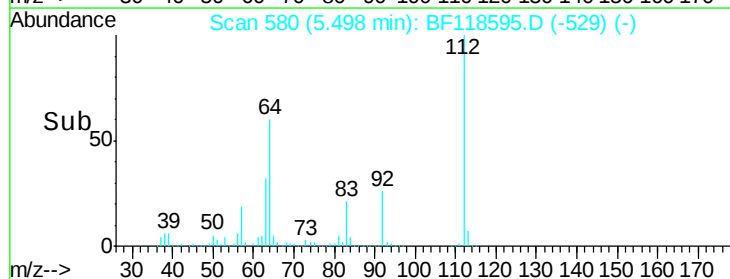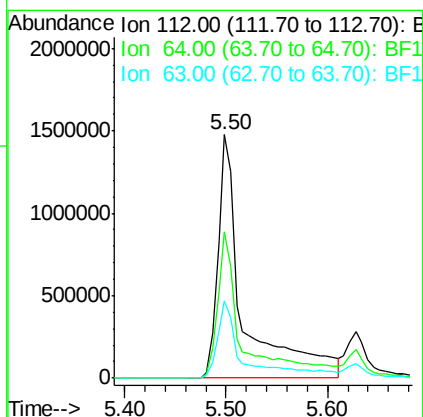



#7

Phenol-d6

Concen: 111.958 ng

RT: 6.50 min Scan# 751

Delta R.T. -0.01 min

Lab File: BF118595.D

Acq: 20 Jan 2020 17:07

Instrument :

BNA_F

ClientSampleId :

B3-15-20





Tot Ion: 99 Resp: 3620526

Ion Ratio Lower Upper

99 100

42 19.3 14.2 21.2

71 37.6 27.8 41.6

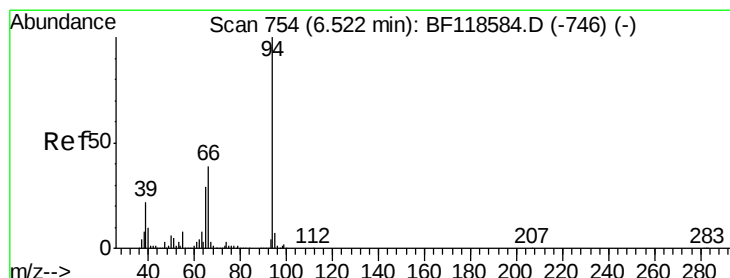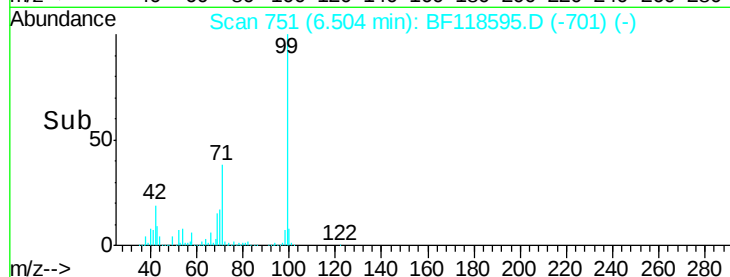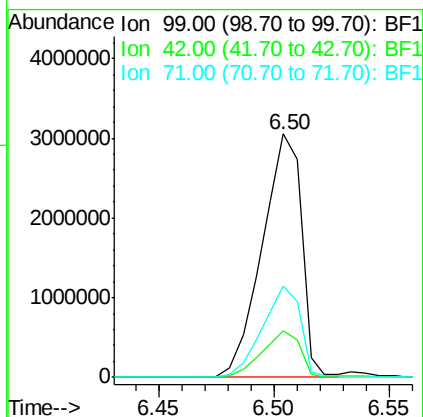

#10

Phenol

Concen: 4.022 ng

RT: 6.52 min Scan# 753

Delta R.T. -0.01 min

Lab File: BF118595.D

Acq: 20 Jan 2020 17:07




Tgt Ion: 94 Resp: 148224

Ion Ratio Lower Upper

94 100

65 28.9 9.5 49.5

66 41.1 18.5 58.5

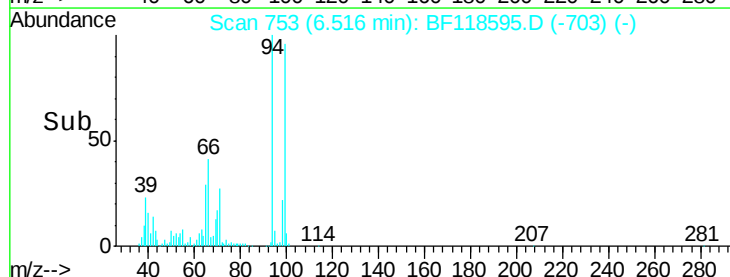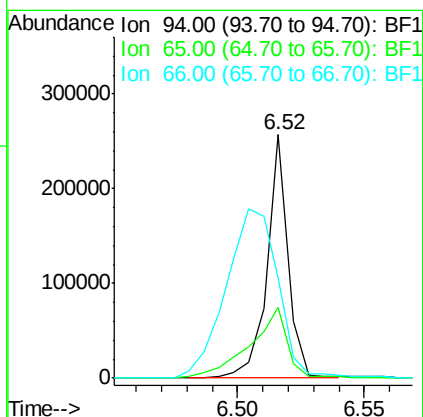



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1033

Delta R.T. -0.01 min

Lab File: BF118595.D

Acq: 20 Jan 2020 17:07

Instrument :

BNA_F

ClientSampleId :

B3-15-20

Tot Ion:136 Resp: 1686385



Ion Ratio Lower Upper

136 100

137 11.5 9.1 13.7

54 7.1 5.8 8.6

68 6.0 5.0 7.4

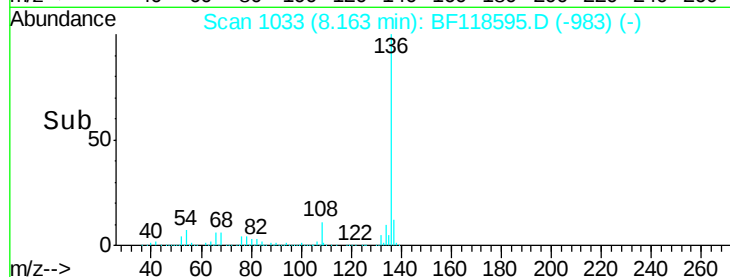
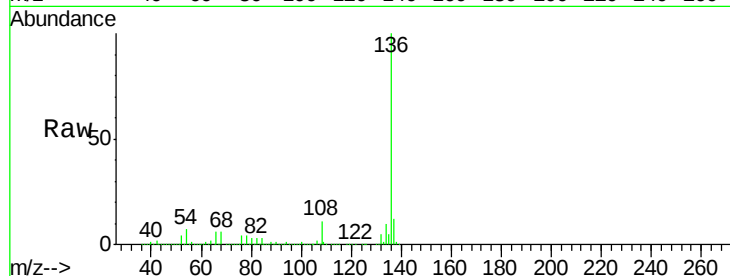


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

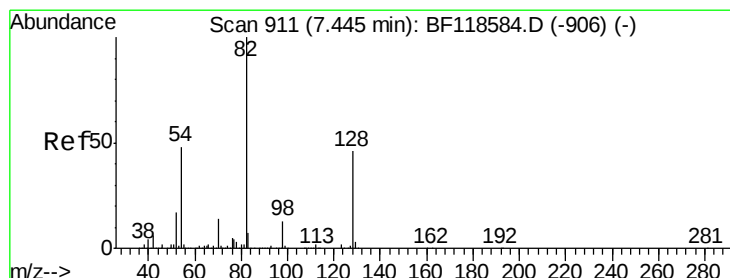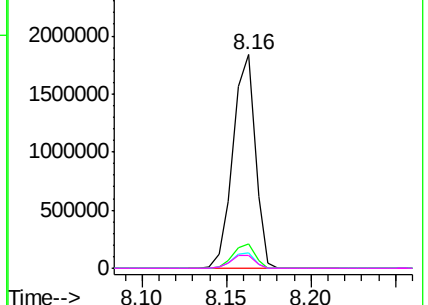

#23

Nitrobenzene-d5

Concen: 75.664 ng

RT: 7.44 min Scan# 910

Delta R.T. -0.01 min

Lab File: BF118595.D

Acq: 20 Jan 2020 17:07



Tgt Ion: 82 Resp: 2281239

Ion Ratio Lower Upper

82 100

128 48.2 36.6 54.8


54 46.1 38.0 57.0

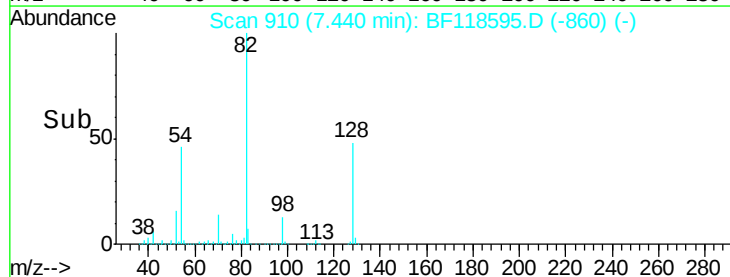


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

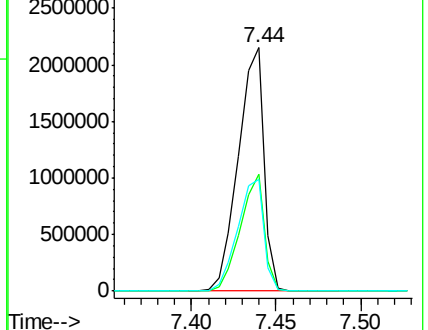

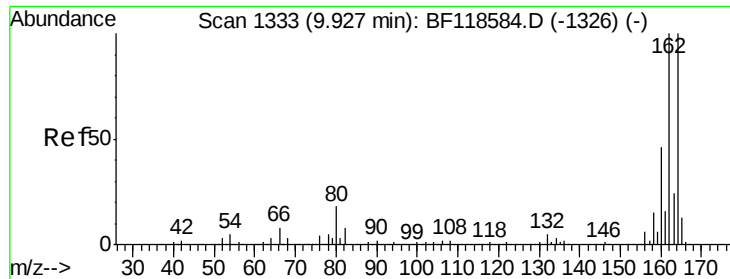

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.92 min Scan# 1331

Delta R.T. -0.01 min

Lab File: BF118595.D

Acq: 20 Jan 2020 17:07

Instrument :

BNA_F

ClientSampled :

B3-15-20


Tot Ion:164 Resp: 969504

Ion Ratio Lower Upper

164 100

162 101.8 80.4 120.6




160 46.6 36.6 55.0



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

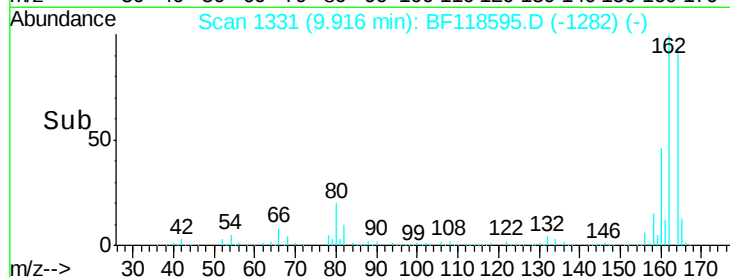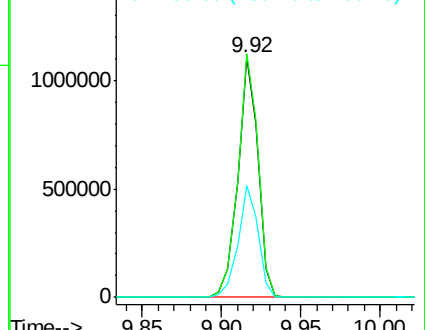

#42

2,4,6-Tribromophenol

Concen: 113.941 ng

RT: 10.70 min Scan# 1465

Delta R.T. -0.01 min

Lab File: BF118595.D

Acq: 20 Jan 2020 17:07


Tgt Ion:330 Resp: 1277678

Ion Ratio Lower Upper

330 100

332 95.6 76.2 114.4



141 28.9 23.9 35.9




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

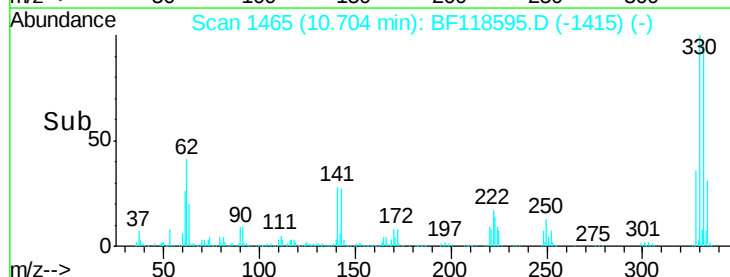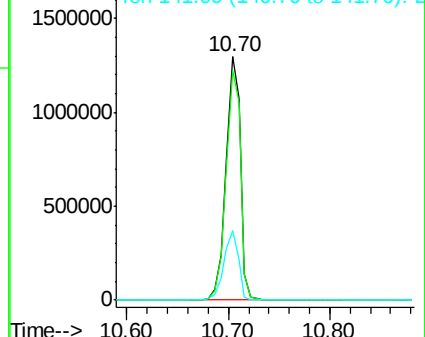


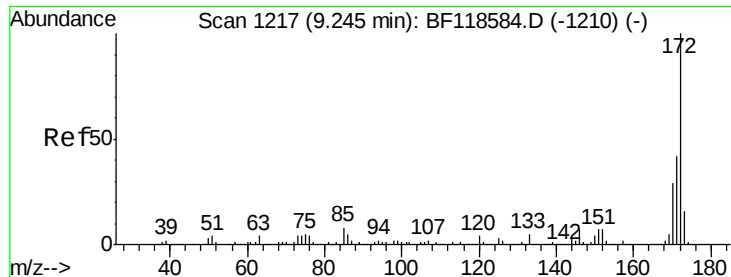




#45
2-Fluorobiphenyl
Concen: 70.233 ng
RT: 9.24 min Scan# 1216
Delta R.T. -0.01 min
Lab File: BF118595.D
Acq: 20 Jan 2020 17:07

Instrument :
BNA_F
ClientSampled :
B3-15-20

Tot Ion:172 Resp: 4142744
Ion Ratio Lower Upper
172 100
171 40.7 33.4 50.2
170 28.2 23.2 34.8

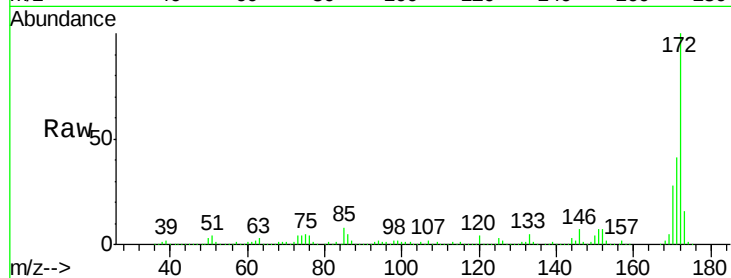


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

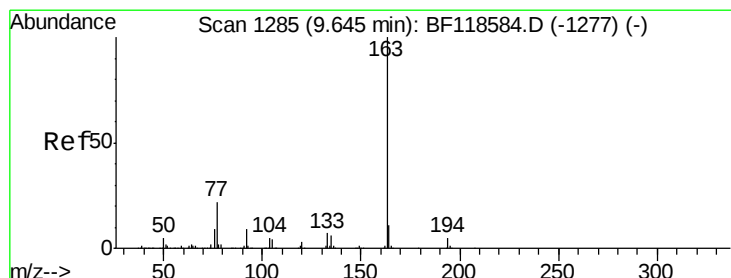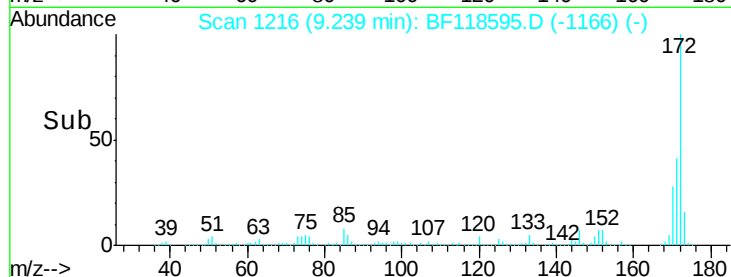
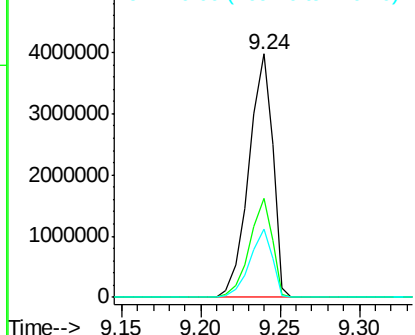



#50
Dimethylphthalate
Concen: 6.045 ng
RT: 9.63 min Scan# 1282
Delta R.T. -0.02 min
Lab File: BF118595.D
Acq: 20 Jan 2020 17:07

Tgt Ion:163 Resp: 381843
Ion Ratio Lower Upper
163 100
194 4.4 3.9 5.9
164 10.1 9.1 13.7

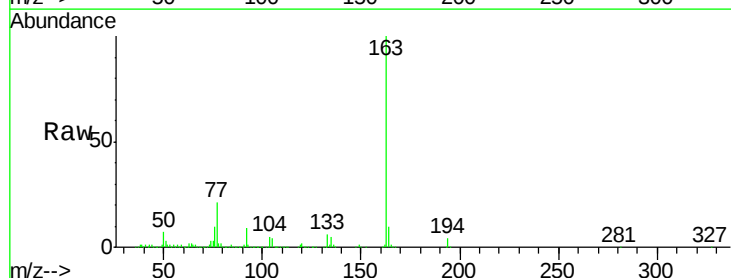

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



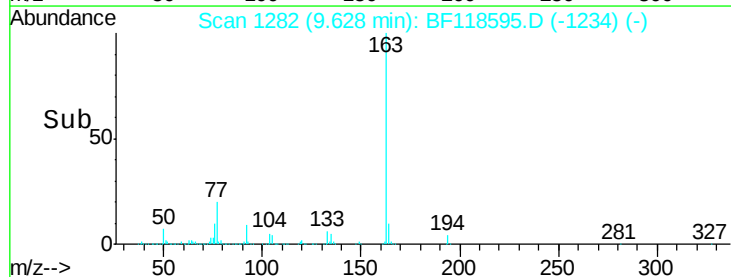
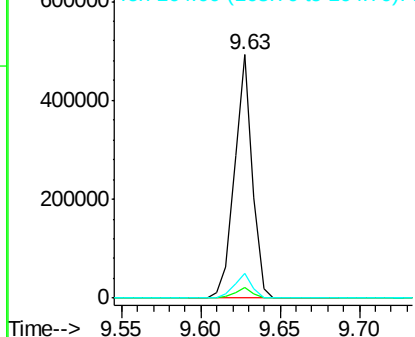


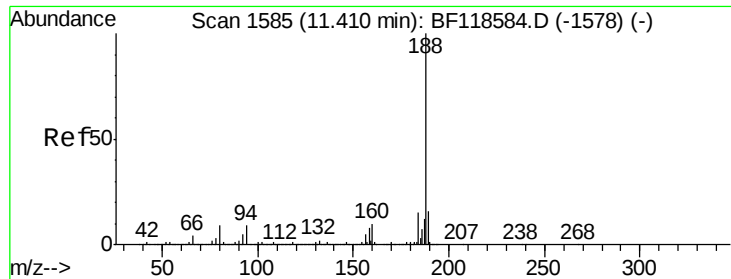

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. -0.01 min
Lab File: BF118595.D
Acq: 20 Jan 2020 17:07




Instrument :
BNA_F
ClientSampled :
B3-15-20


Tot Ion:188 Resp: 1770612
Ion Ratio Lower Upper
188 100
94 8.8 7.1 10.7
80 9.2 7.5 11.3

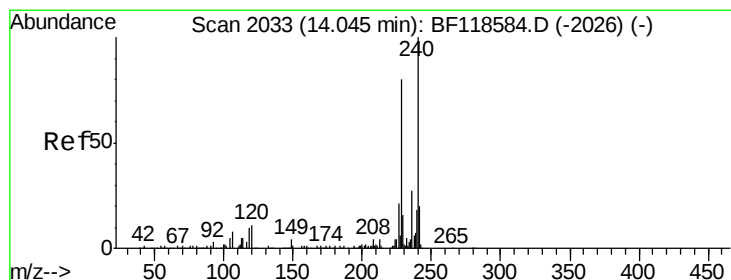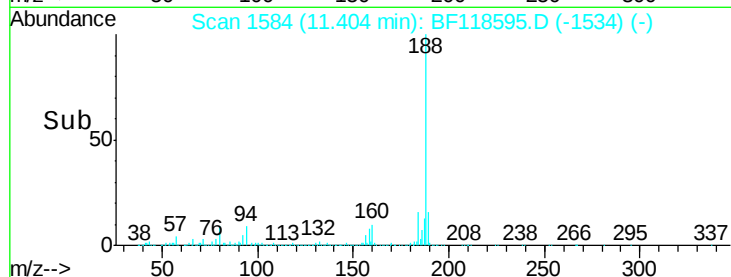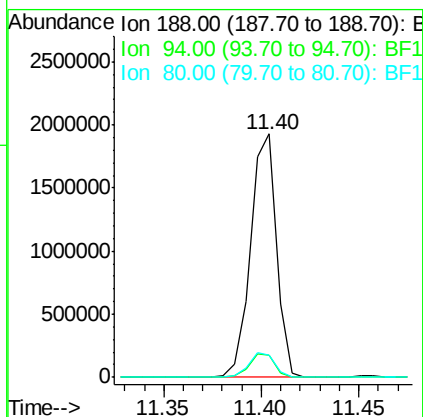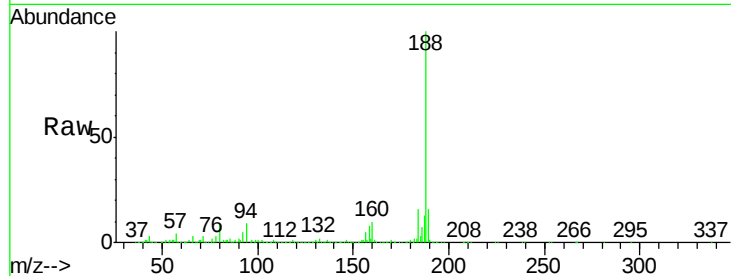

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.04 min Scan# 2032
Delta R.T. -0.01 min
Lab File: BF118595.D
Acq: 20 Jan 2020 17:07

Tgt Ion:240 Resp: 1152666
Ion Ratio Lower Upper
240 100
120 9.2 8.9 13.3
236 26.7 21.5 32.3

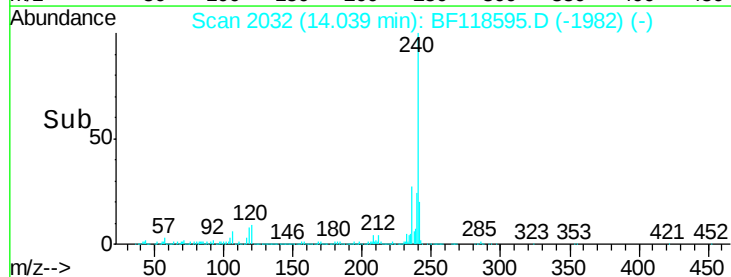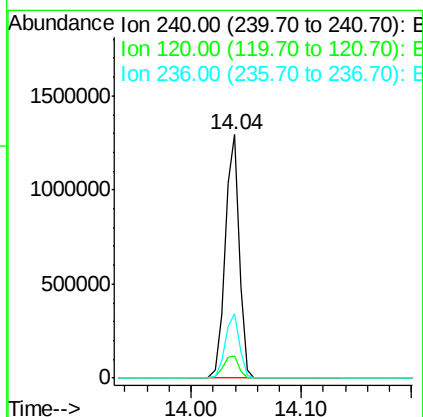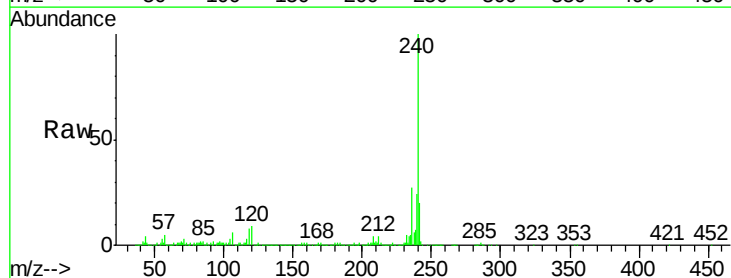

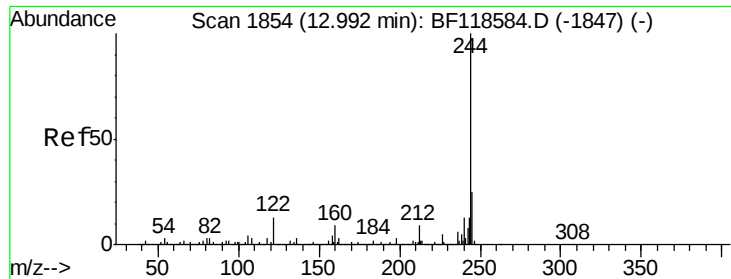

#79

Terphenyl-d14

Concen: 88.829 ng

RT: 12.99 min Scan# 1854

Delta R.T. 0.00 min

Lab File: BF118595.D

Acq: 20 Jan 2020 17:07

Instrument :

BNA_F

ClientSampled :

B3-15-20


Tot Ion:244 Resp: 4694440

Ion Ratio Lower Upper

244 100

212 8.8 7.0 10.4




122 12.1 10.7 16.1

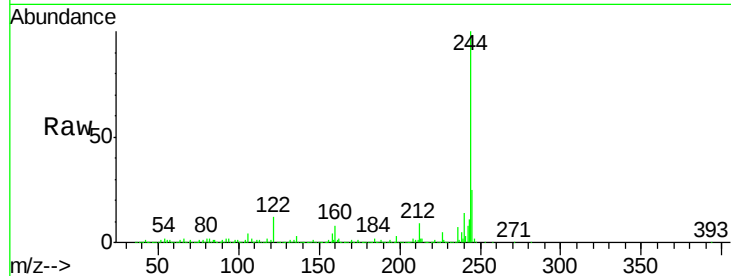

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

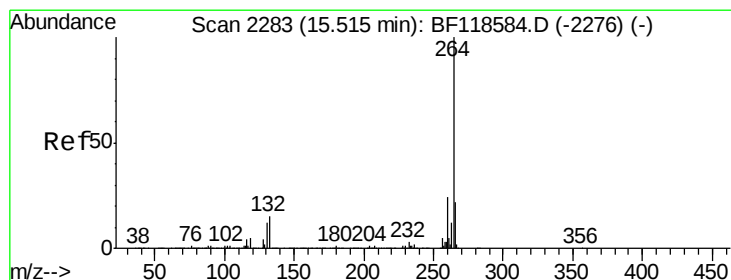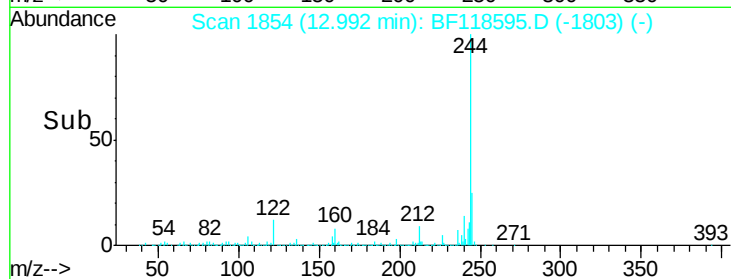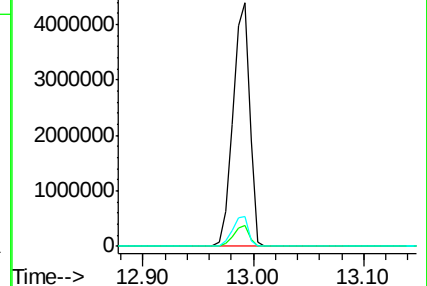

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.51 min Scan# 2282

Delta R.T. -0.01 min

Lab File: BF118595.D

Acq: 20 Jan 2020 17:07


Tgt Ion:264 Resp: 1077401

Ion Ratio Lower Upper

264 100

260 24.8 19.6 29.4

265 22.6 17.7 26.5

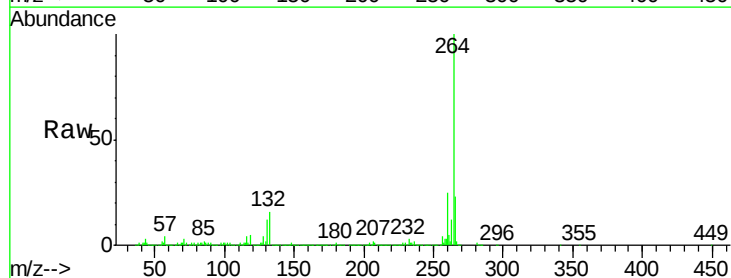

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

