


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012020\
 Data File : BF118591.D
 Acq On : 20 Jan 2020 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 20 14:45:03 2020

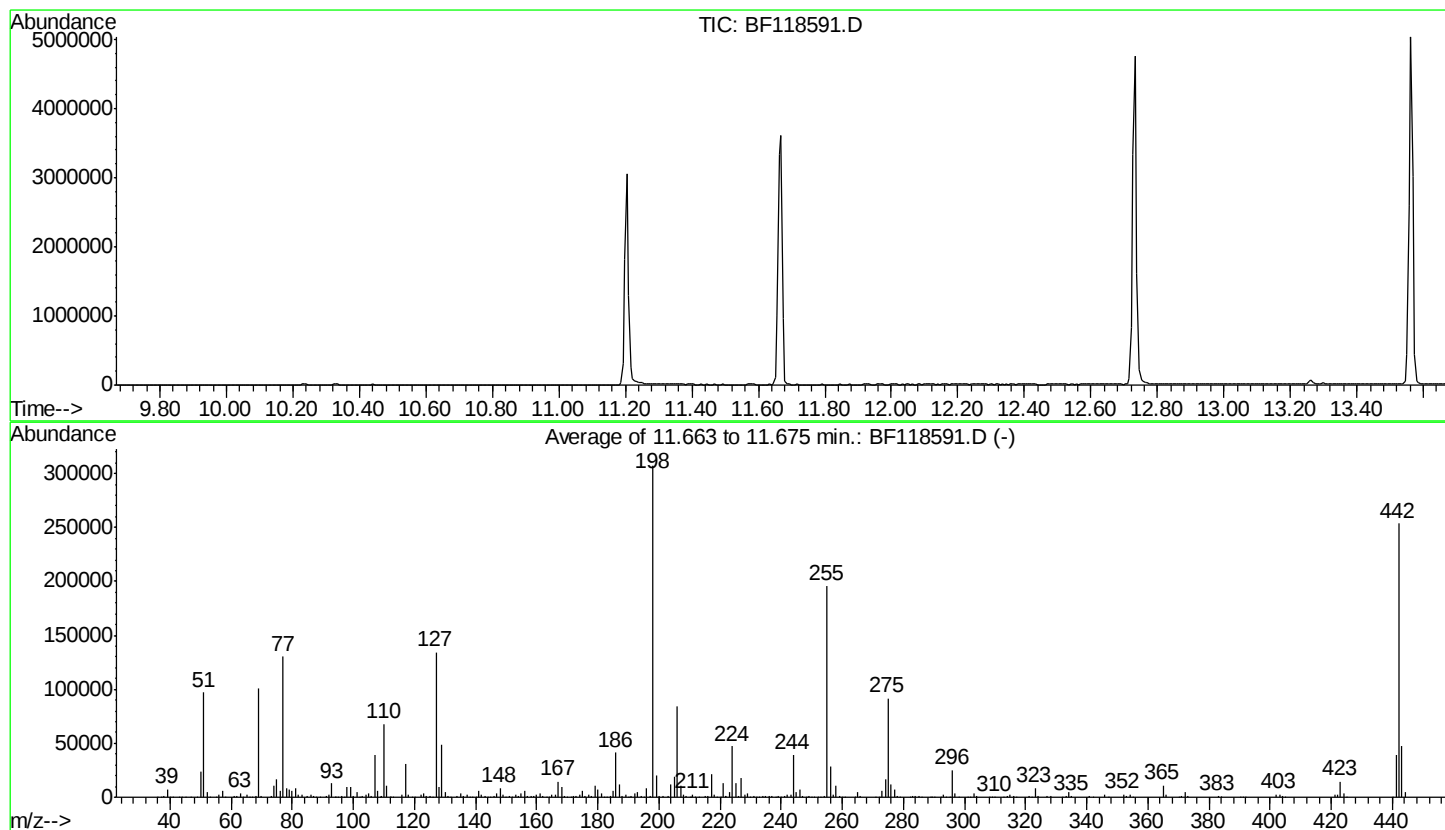

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	97107	PASS
68	69	0.00	2	1.8	1769	PASS
69	198	0.00	100	32.9	101029	PASS
70	69	0.00	2	0.7	664	PASS
127	198	10	80	43.7	134213	PASS
197	198	0.00	2	0.5	1470	PASS
198	198	100	100	100.0	307360	PASS
199	198	5	9	6.7	20463	PASS
275	198	10	60	29.8	91560	PASS
365	198	1	100	3.5	10756	PASS
441	198	0.01	100	12.8	39378	PASS
442	198	50	100	82.5	253482	PASS
443	442	15	24	18.6	47216	PASS