

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012022\
 Data File : BF126613.D
 Acq On : 20 Jan 2022 16:18
 Operator : CG/JU
 Sample : M5190-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CHRT-26598

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.098	166	172	178	rVB	190913	266332	4.58%	0.775%
2	4.810	458	463	467	rBV	369355	373498	6.43%	1.087%
3	5.228	529	534	539	rVB2	325170	469832	8.08%	1.367%
4	5.598	591	597	600	rBV	3447213	3741244	64.37%	10.886%
5	6.581	758	764	767	rBV	3438770	3564785	61.33%	10.373%
6	6.963	826	829	833	rBV	894383	715439	12.31%	2.082%
7	7.528	917	925	928	rBV	2823440	2789377	47.99%	8.116%
8	7.586	928	935	939	rVB	61289	78870	1.36%	0.229%
9	8.245	1043	1047	1050	rBV	1138493	947266	16.30%	2.756%
10	8.910	1154	1160	1163	rBV	72555	64378	1.11%	0.187%
11	9.322	1225	1230	1233	rBV	4309094	4264716	73.38%	12.409%
12	10.004	1342	1346	1349	rVB	1340277	1048522	18.04%	3.051%
13	10.127	1362	1367	1374	rBV	120827	108177	1.86%	0.315%
14	10.357	1399	1406	1412	rBV	166209	158766	2.73%	0.462%
15	10.798	1475	1481	1484	rBV	3051010	2868805	49.36%	8.347%
16	11.410	1575	1585	1588	rBV	4040984	5812016	100.00%	16.911%
17	11.498	1597	1600	1603	rVB	1368032	1079609	18.58%	3.141%
18	12.763	1812	1815	1819	rVB	171245	135645	2.33%	0.395%
19	13.092	1865	1871	1874	rBV	4778262	4540459	78.12%	13.211%
20	14.145	2046	2050	2054	rVB	885753	748216	12.87%	2.177%
21	15.674	2305	2310	2315	rBV	470695	591612	10.18%	1.721%




Sum of corrected areas: 34367564

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012022\
Data File : BF126613.D
Acq On : 20 Jan 2022 16:18
Operator : CG/JU
Sample : M5190-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CHRT-26598

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

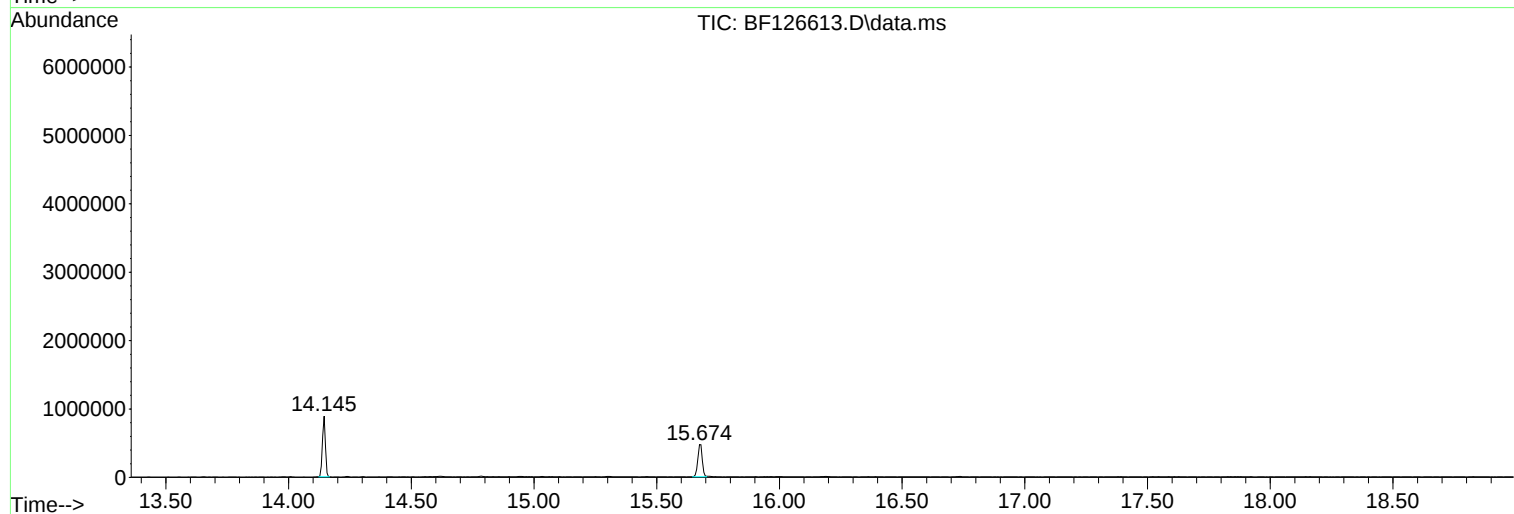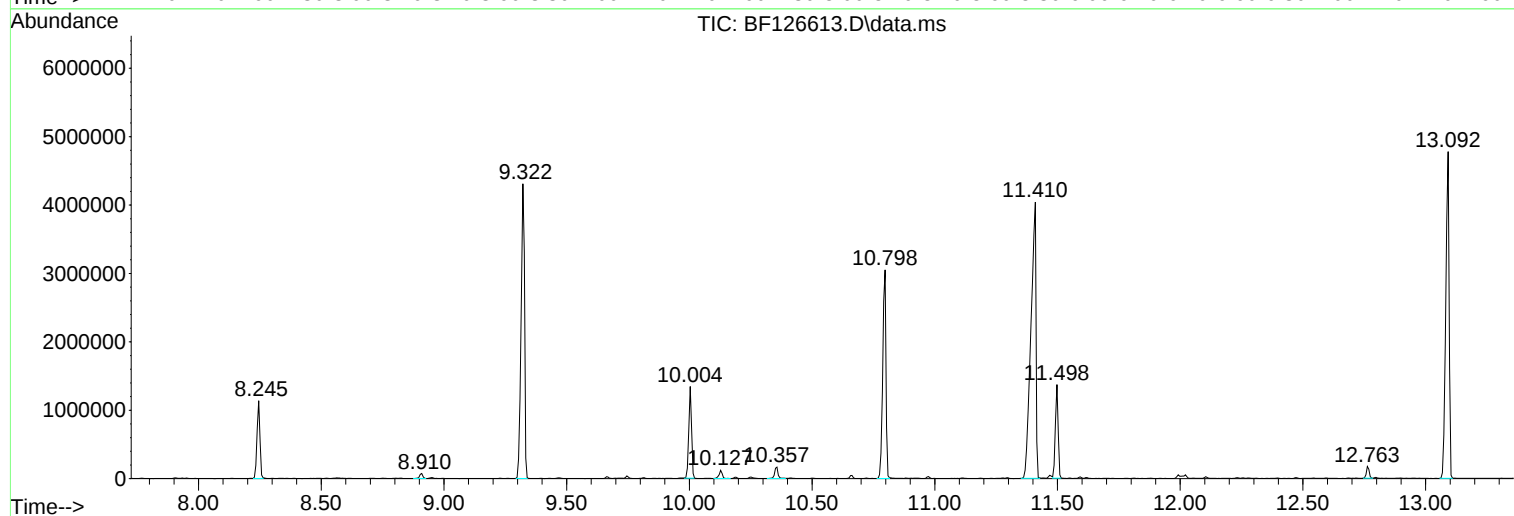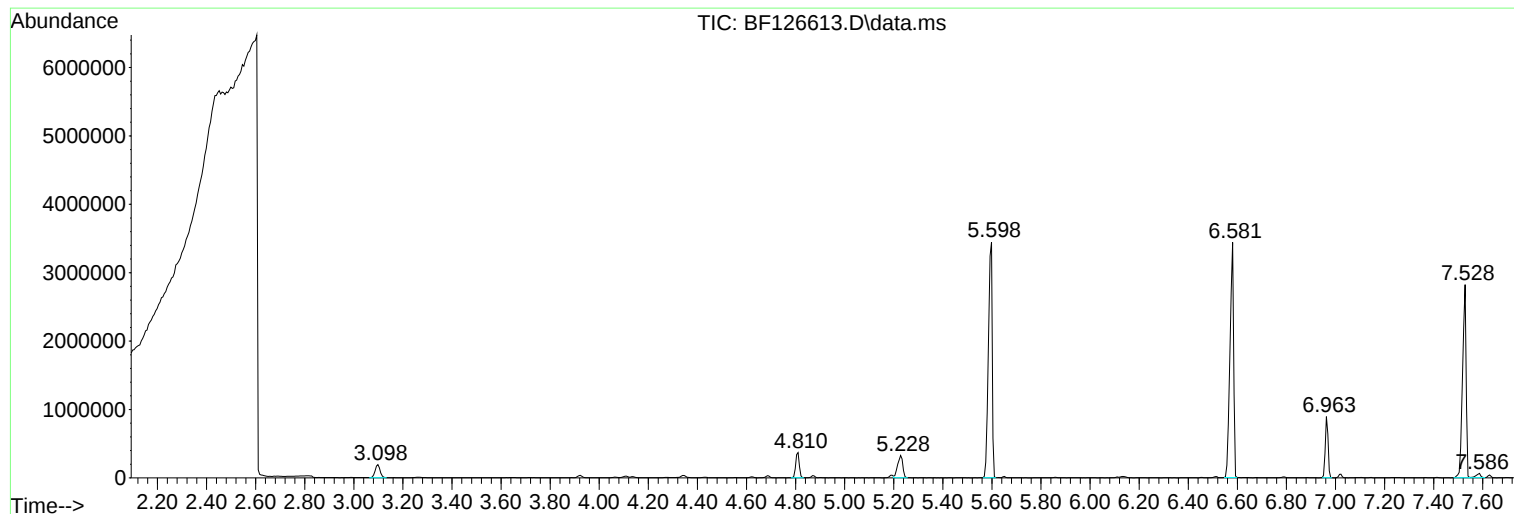

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012022\
Data File : BF126613.D
Acq On : 20 Jan 2022 16:18
Operator : CG/JU
Sample : M5190-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CHRT-26598

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012022\
Data File : BF126613.D
Acq On : 20 Jan 2022 16:18
Operator : CG/JU
Sample : M5190-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CHRT-26598

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------