
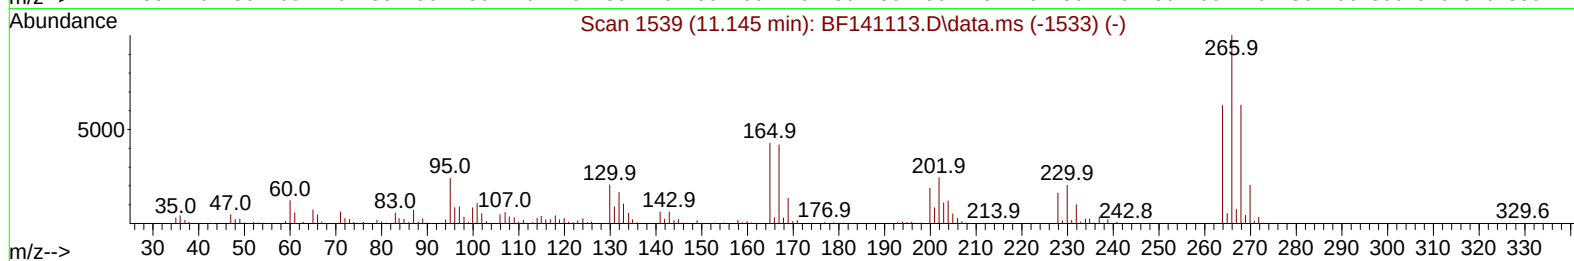
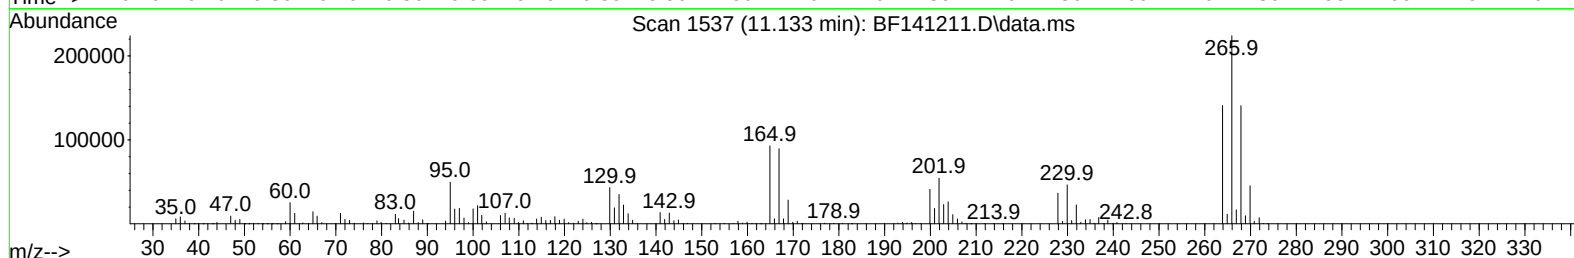


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012025\
Data File : BF141211.D
Acq On : 20 Jan 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 10:54:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

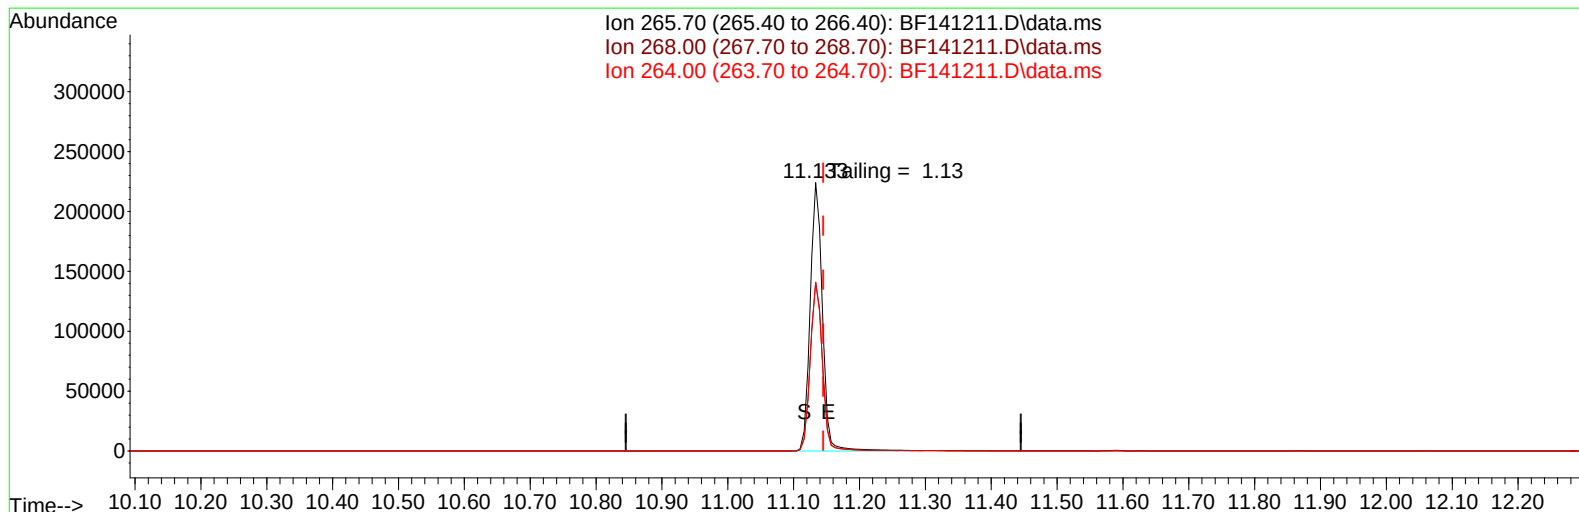

TIC: BF141211.D\data.ms

(70) Pentachlorophenol (C)




11.133min (-0.012) 44495.62 ng

response 289966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.84
264.00	62.70	62.90
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012025\  
Data File : BF141211.D  
Acq On    : 20 Jan 2025 09:40  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jan 20 10:54:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

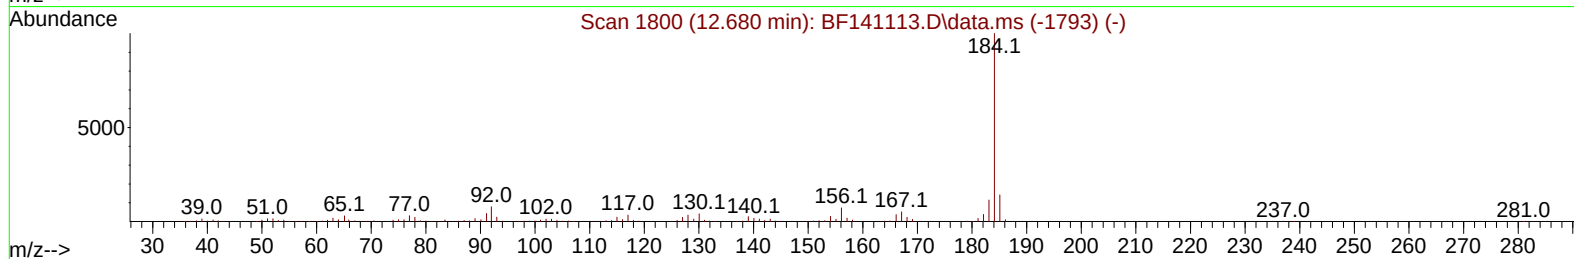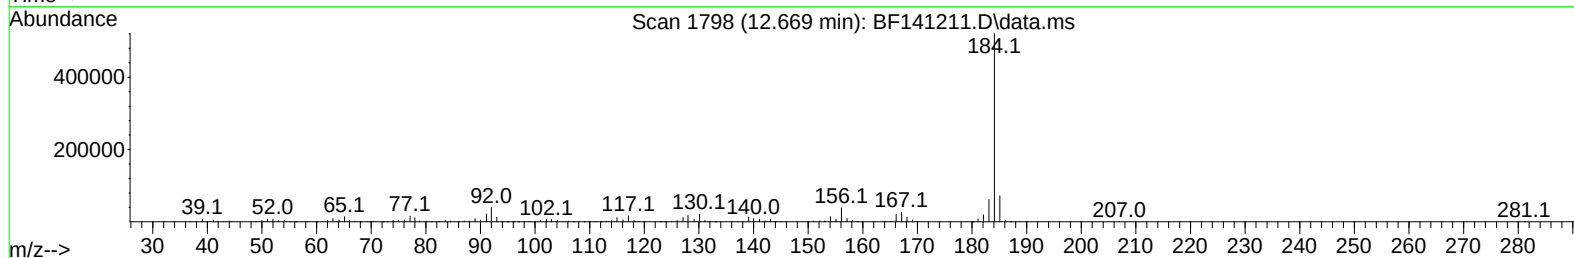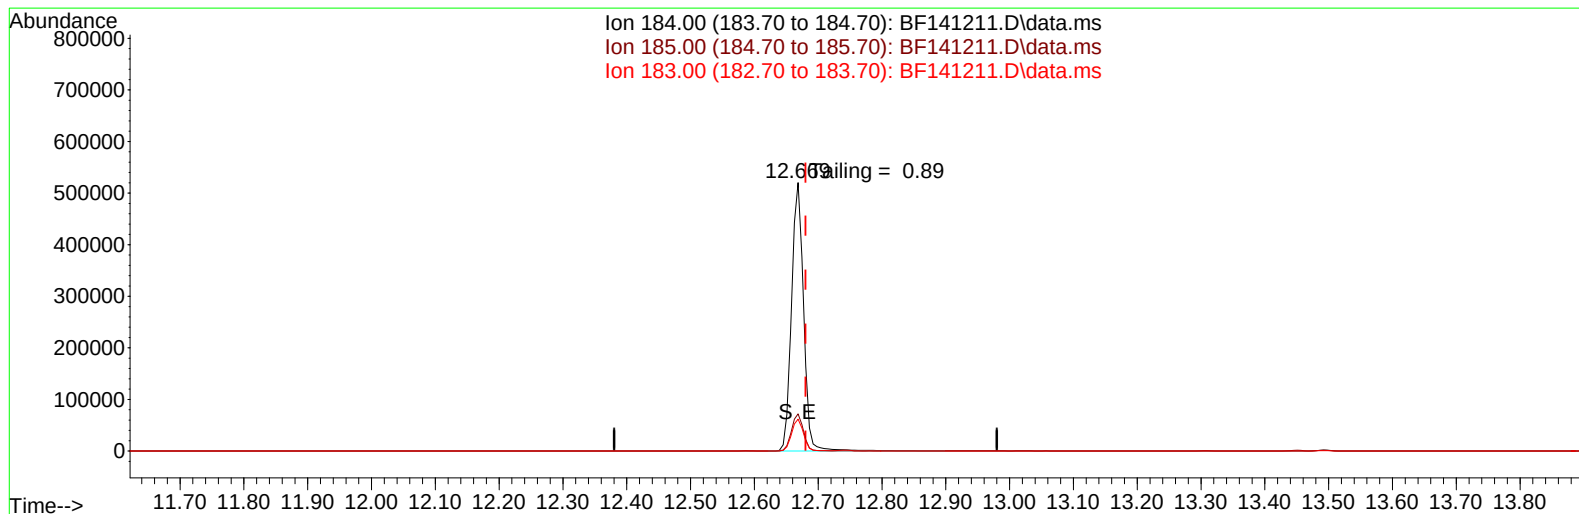

TIC: BF141211.D\data.ms

(77) Benzidine

12.669min (-0.012) 48437.63 ng

response **683565**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.84
183.00	11.50	11.90
0.00	0.00	0.00