

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012115\
 Data File : BF077006.D
 Acq On : 21 Jan 2015 20:59
 Operator : TP/IZ
 Sample : G1118-05
 Misc : GPC-BLK
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.430	28	30	41	rBV	39500	93549	39.89%	6.394%
2	7.853	589	592	597	rVB	86747	137284	58.54%	9.383%
3	10.756	843	846	850	rBV	125828	201660	85.99%	13.782%
4	14.883	1204	1207	1211	rBV	137511	225390	96.11%	15.404%
5	17.694	1450	1453	1455	rBV	169972	232222	99.02%	15.871%
6	21.192	1756	1759	1761	rBV	187044	234522	100.00%	16.028%
7	22.826	1899	1902	1905	rBV	170360	219559	93.62%	15.006%
8	22.895	1906	1908	1912	rBV2	1543	2854	1.22%	0.195%
9	23.112	1924	1927	1928	rBV2	2094	3222	1.37%	0.220%
10	23.283	1940	1942	1944	rBV3	2115	3116	1.33%	0.213%
11	23.398	1949	1952	1953	rBV3	2069	3014	1.29%	0.206%
12	23.752	1979	1983	1986	rBV4	2830	10681	4.55%	0.730%
13	23.843	1990	1991	1993	rVB2	2244	2829	1.21%	0.193%
14	23.889	1993	1995	1997	rBV3	1727	3589	1.53%	0.245%
15	24.083	2010	2012	2013	rBV	3839	6371	2.72%	0.435%
16	24.278	2028	2029	2032	rBV3	1981	3592	1.53%	0.245%
17	24.586	2053	2056	2058	rBV4	2758	5534	2.36%	0.378%
18	24.644	2058	2061	2063	rBV4	2110	6071	2.59%	0.415%
19	24.769	2069	2072	2075	rBV3	2431	5993	2.56%	0.410%
20	24.815	2075	2076	2078	rBV2	3448	4154	1.77%	0.284%
21	25.226	2111	2112	2115	rBV2	2224	3596	1.53%	0.246%
22	25.627	2146	2147	2151	rVB3	2755	5521	2.35%	0.377%
23	25.706	2151	2154	2156	rBV3	2702	6455	2.75%	0.441%
24	26.141	2188	2192	2193	rBV3	2573	7010	2.99%	0.479%
25	26.335	2206	2209	2214	rBV6	2978	9169	3.91%	0.627%
26	26.404	2214	2215	2218	rVB3	2627	3825	1.63%	0.261%
27	26.484	2221	2222	2223	rBV	2789	2519	1.07%	0.172%
28	26.518	2223	2225	2227	rVB3	1989	2787	1.19%	0.190%
29	26.632	2233	2235	2237	rBV3	2154	3783	1.61%	0.259%
30	26.838	2249	2253	2254	rBV3	2106	3707	1.58%	0.253%
31	27.124	2274	2278	2281	rVB4	2300	6323	2.70%	0.432%
32	27.238	2286	2288	2289	rBV2	2160	3287	1.40%	0.225%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012115\
Data File : BF077006.D
Acq On : 21 Jan 2015 20:59
Operator : TP/IZ
Sample : G1118-05
Misc : GPC-BLK
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 1463188

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012115\
Data File : BF077006.D
Acq On : 21 Jan 2015 20:59
Operator : TP/IZ
Sample : G1118-05
Misc : GPC-BLK
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

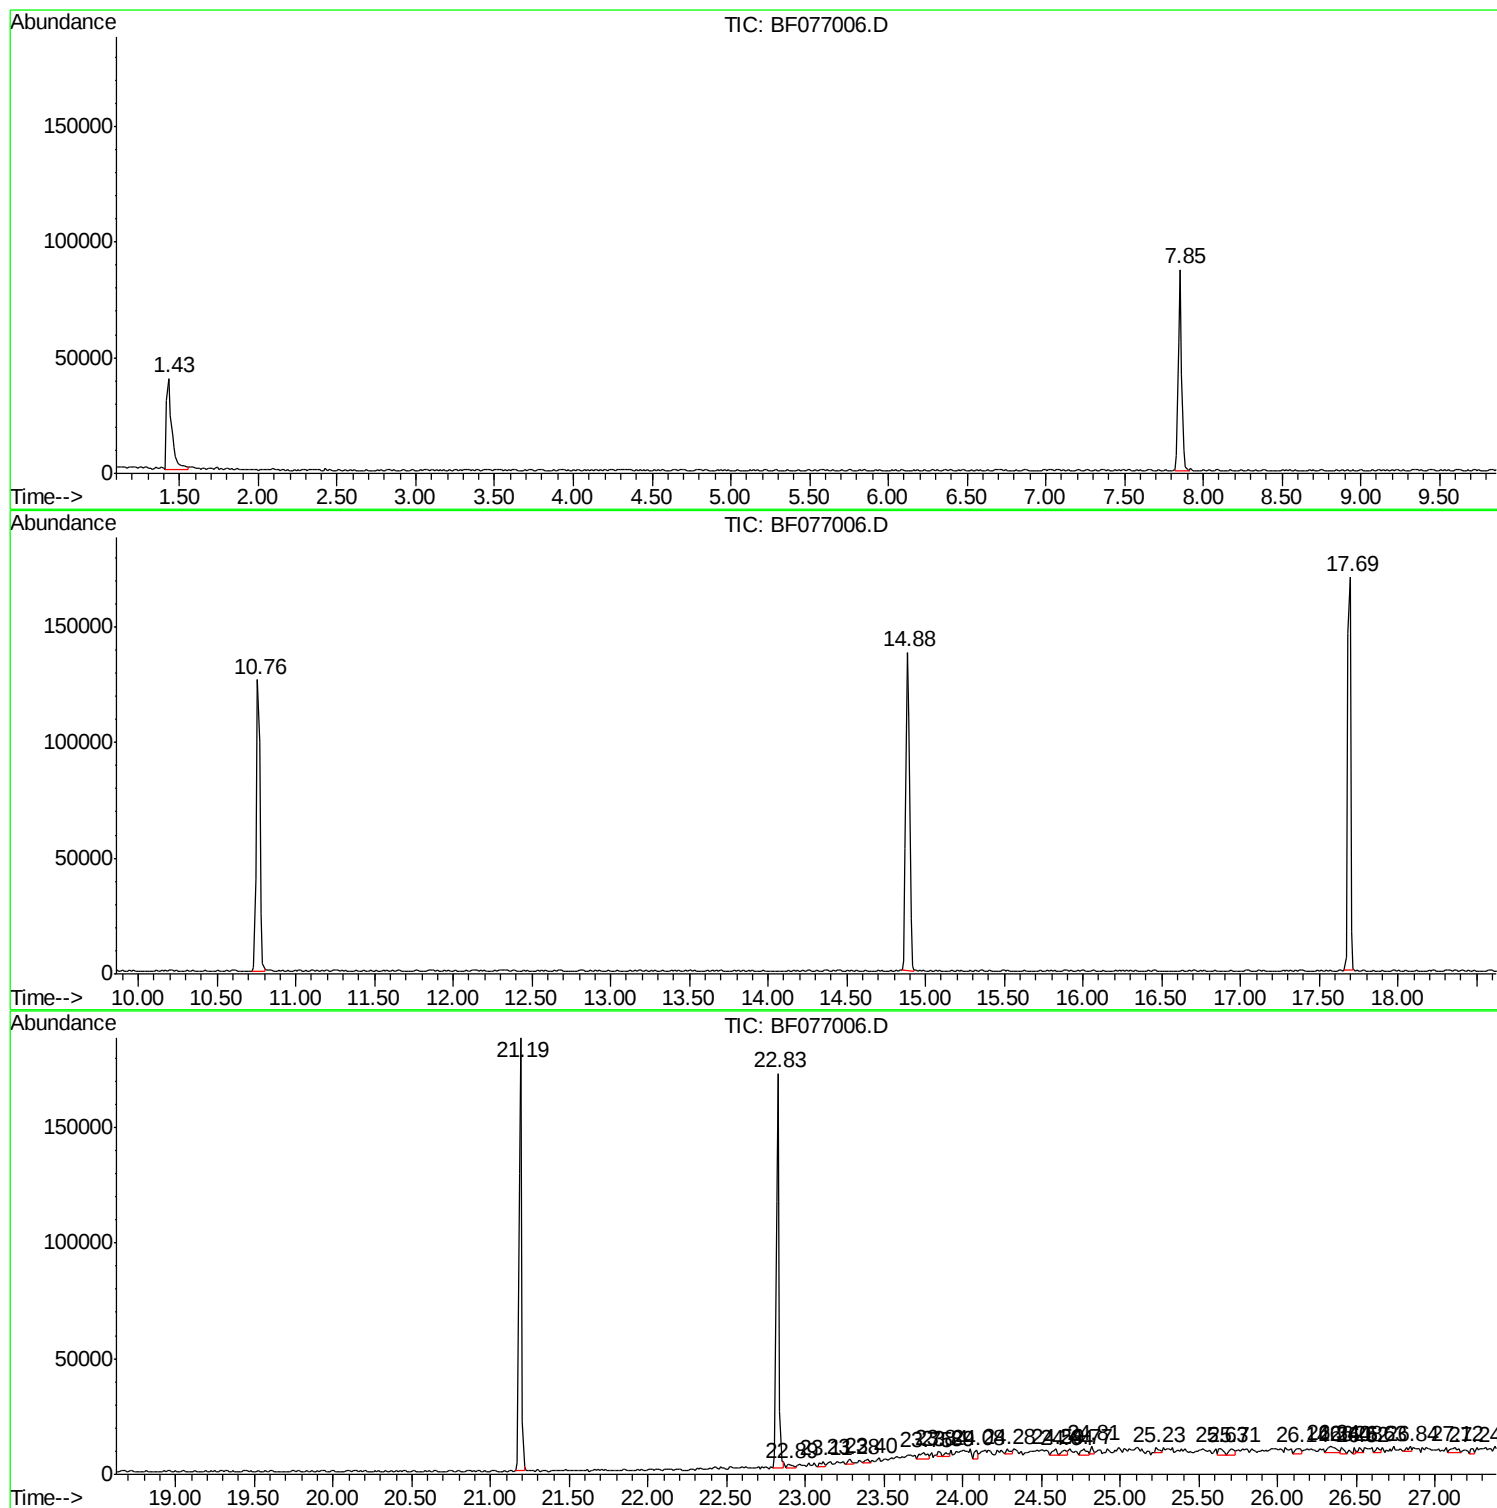

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF012115\
Data_File : BF077006.D
Acq_On : 21-Jan-2015 20:599
Operator : TP/IZZ
Sample : G1118-055
Misc : GPC-BLKK
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
