


Data Path : Z:\HPCHEM1\BNA F\Data\BF012115\
 Data File : BF076994.D
 Acq On : 21 Jan 2015 12:45
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 21 14:45:53 2015

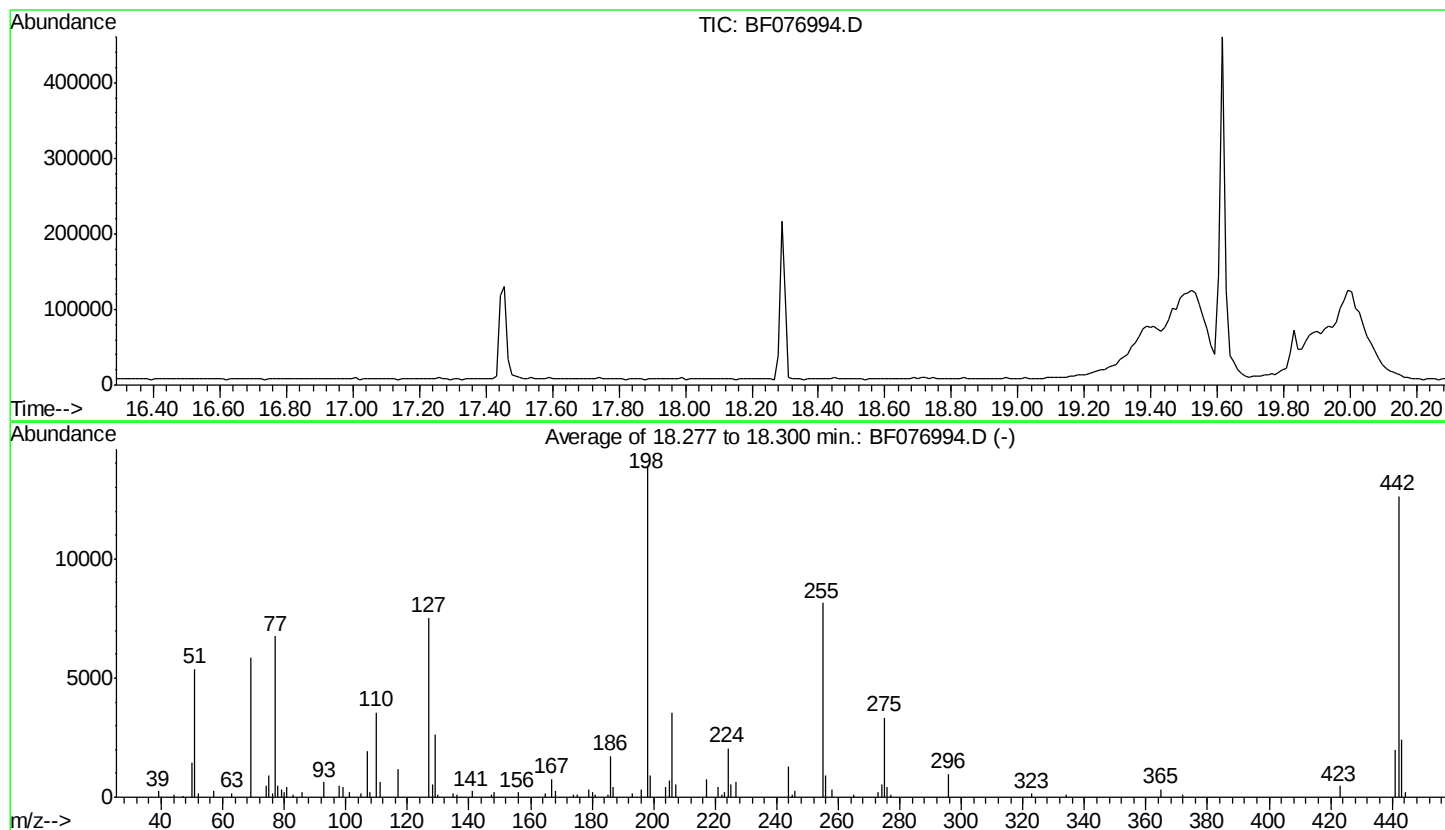

AutoFind: Scans 1504, 1505, 1506; Background Corrected with Scan 1501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	5383	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.2	5876	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.1	7519	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13908	PASS
199	198	5	9	6.5	898	PASS
275	198	10	60	24.0	3333	PASS
365	198	1	100	2.4	339	PASS
441	442	0.01	24	15.7	1980	PASS
442	198	50	100	90.7	12618	PASS
443	442	15	24	19.0	2397	PASS