
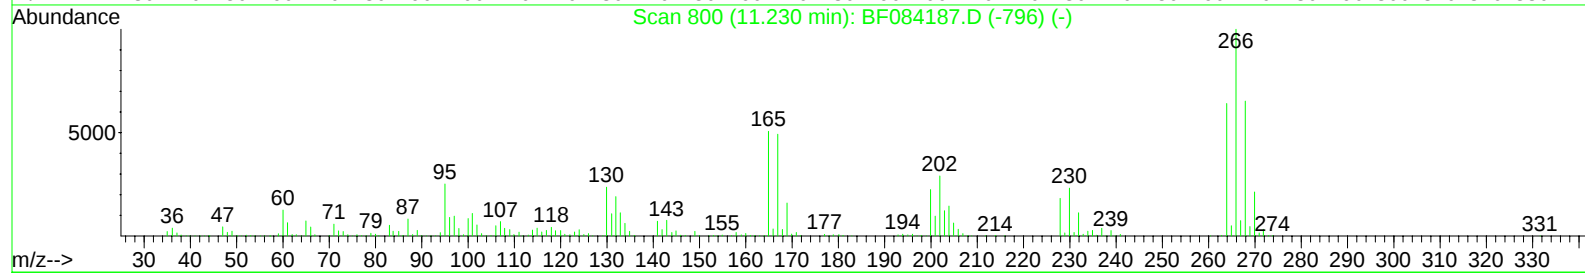
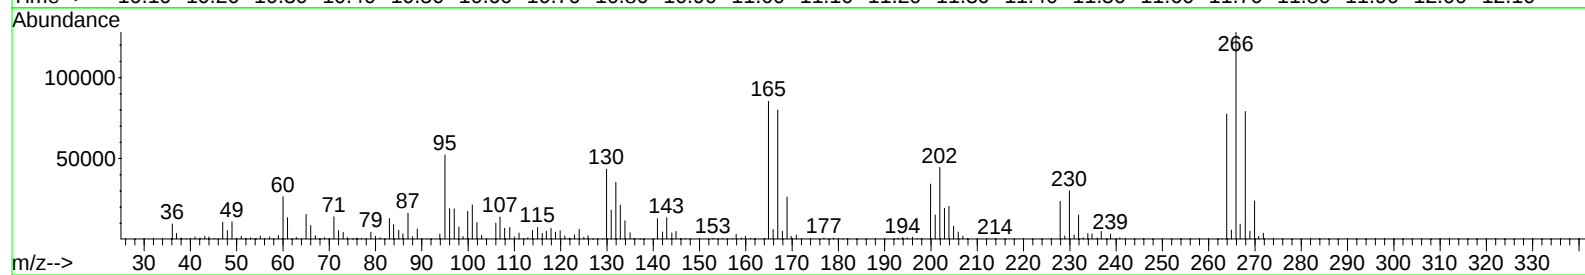


```
Data Path   : Z:\HPCHEM1\BNA F\Data\BF012116\  
Data File  : BF084576.D  
Acq On     : 21 Jan 2016   10:00  
Operator   : SJ/UM  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1      Sample Multiplier: 1
```

Quant Time: Jan 22 06:01:24 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

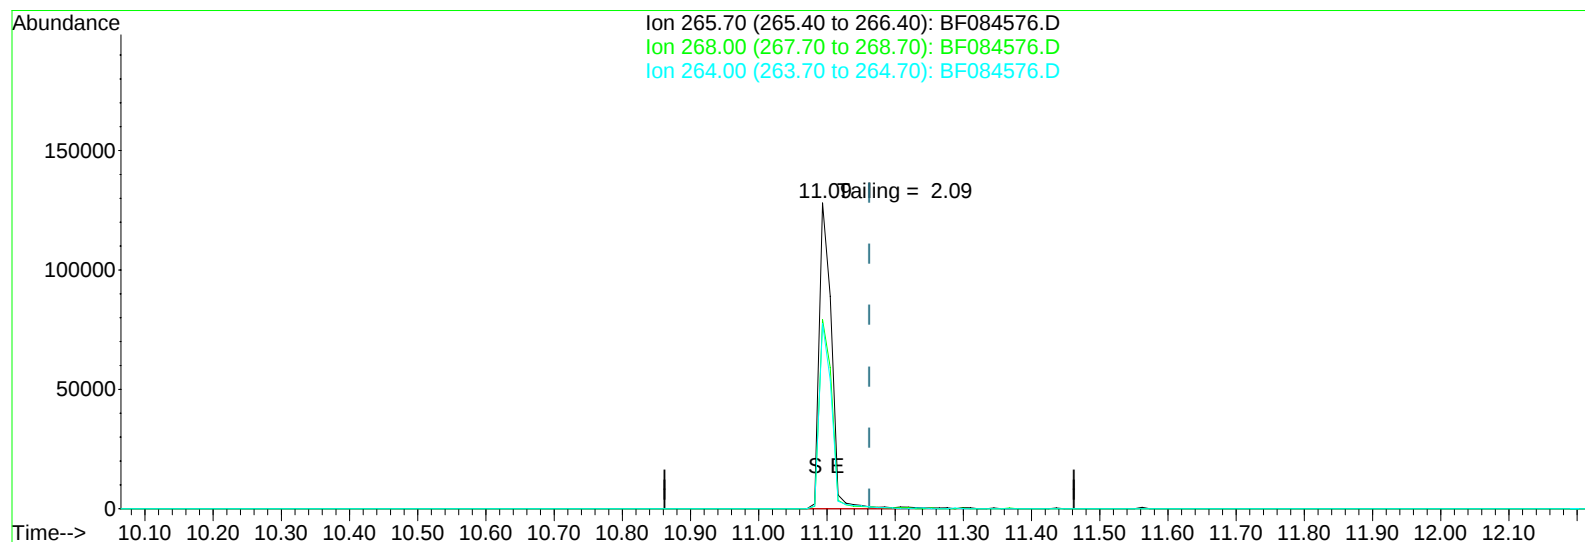

TIC: BF084576.D

(69) Pentachlorophenol (C)




11.093min (-0.069) 0.00ng

response 159801

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	61.80
264.00	62.70	60.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF012116\
Data File : BF084576.D
Acq On : 21 Jan 2016 10:00
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 06:01:24 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

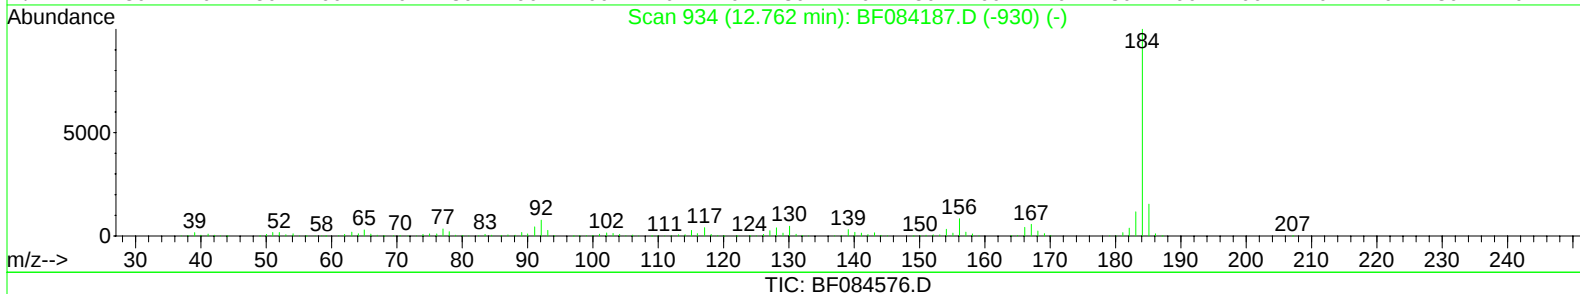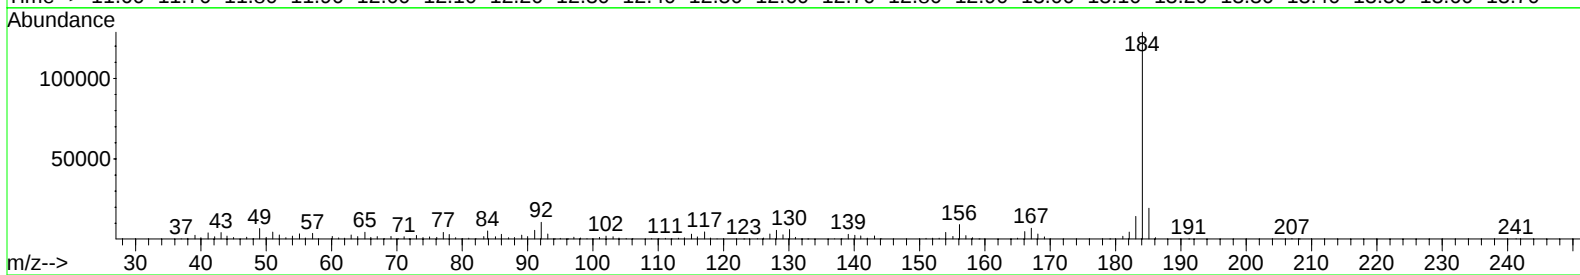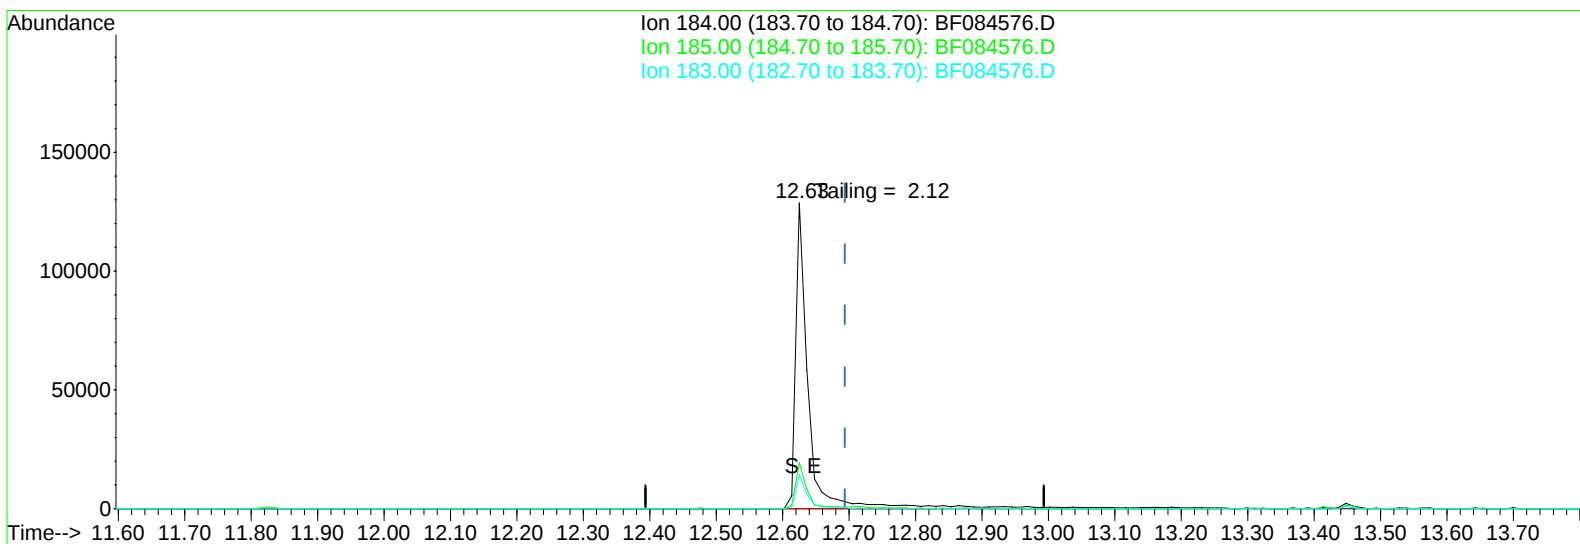

(76) Benzidine

12.625min (-0.069) 509.88ng

response 164389

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.09
183.00	12.30	11.11
0.00	0.00	0.00