


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012116\
 Data File : BF084576.D
 Acq On : 21 Jan 2016 10:00
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 14 14:15:52 2016

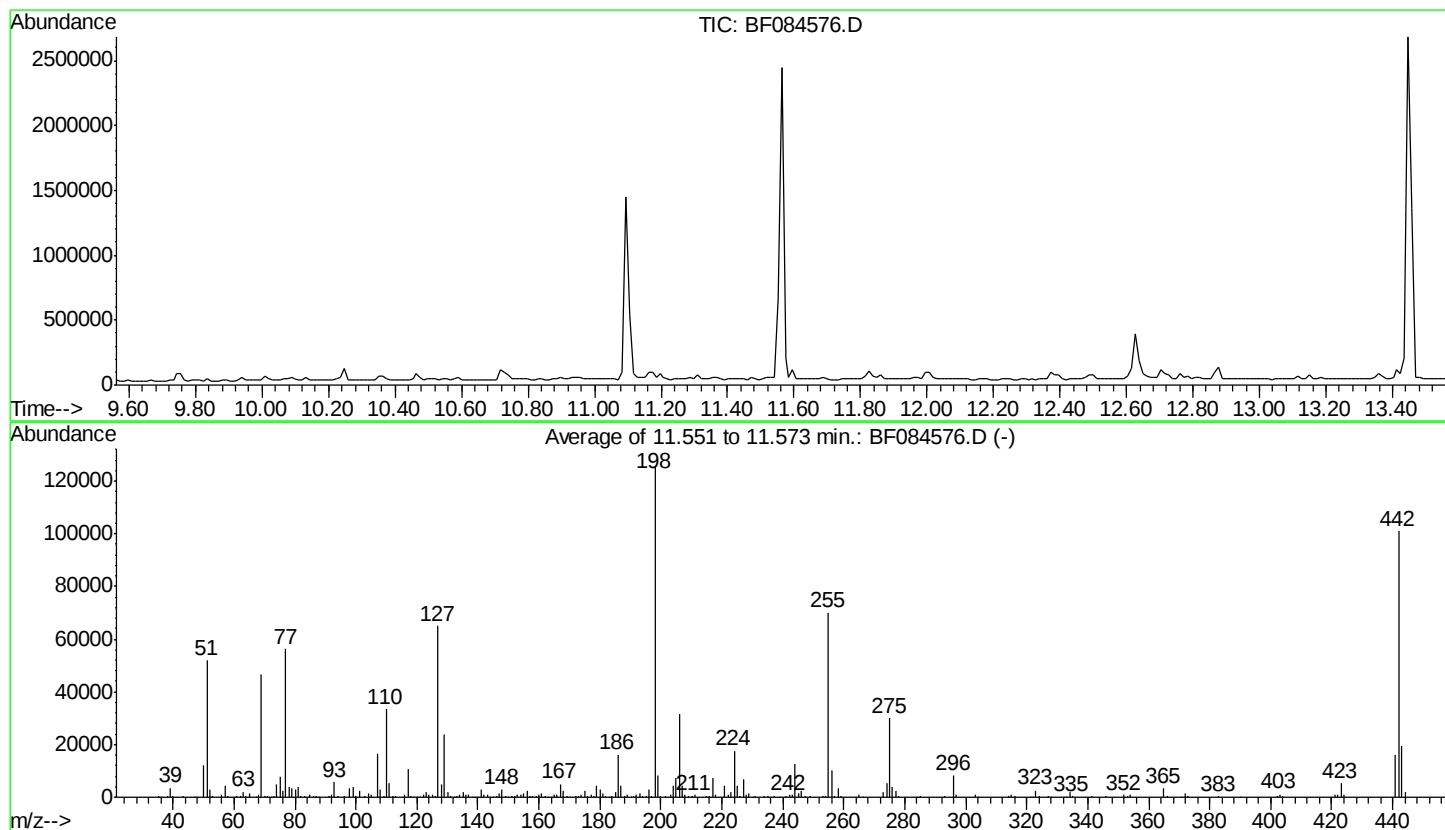

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	51810	PASS
68	69	0.00	2	2.0	915	PASS
69	198	0.00	100	37.1	46679	PASS
70	69	0.00	2	0.8	352	PASS
127	198	10	80	51.5	64881	PASS
197	198	0.00	2	0.6	723	PASS
198	198	100	100	100.0	125866	PASS
199	198	5	9	6.7	8452	PASS
275	198	10	60	23.9	30097	PASS
365	198	1	100	2.7	3406	PASS
441	442	0.01	24	15.8	15915	PASS
442	198	50	100	80.2	100950	PASS
443	442	15	24	19.2	19356	PASS