
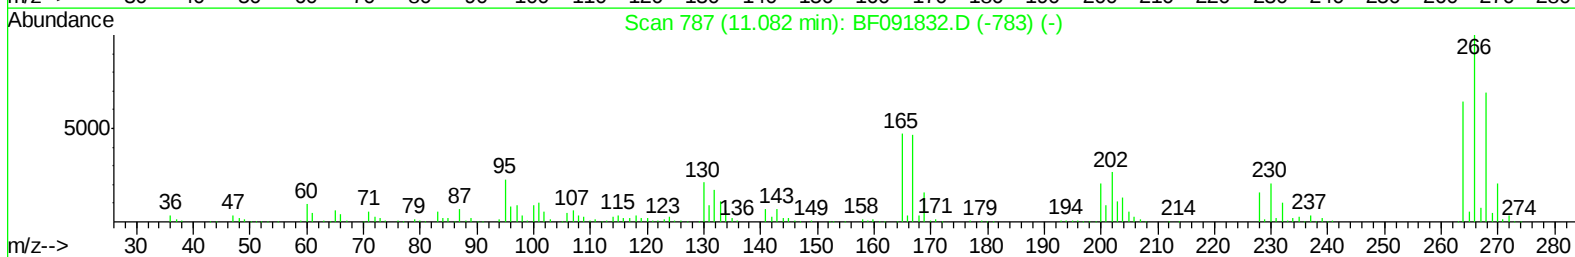
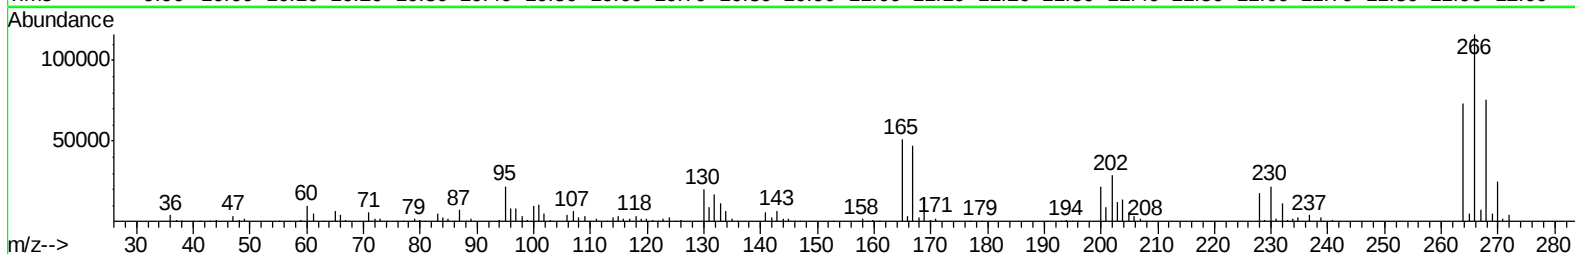


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012117\
Data File : BF092406.D
Acq On : 21 Jan 2017 10:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 07:51:23 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

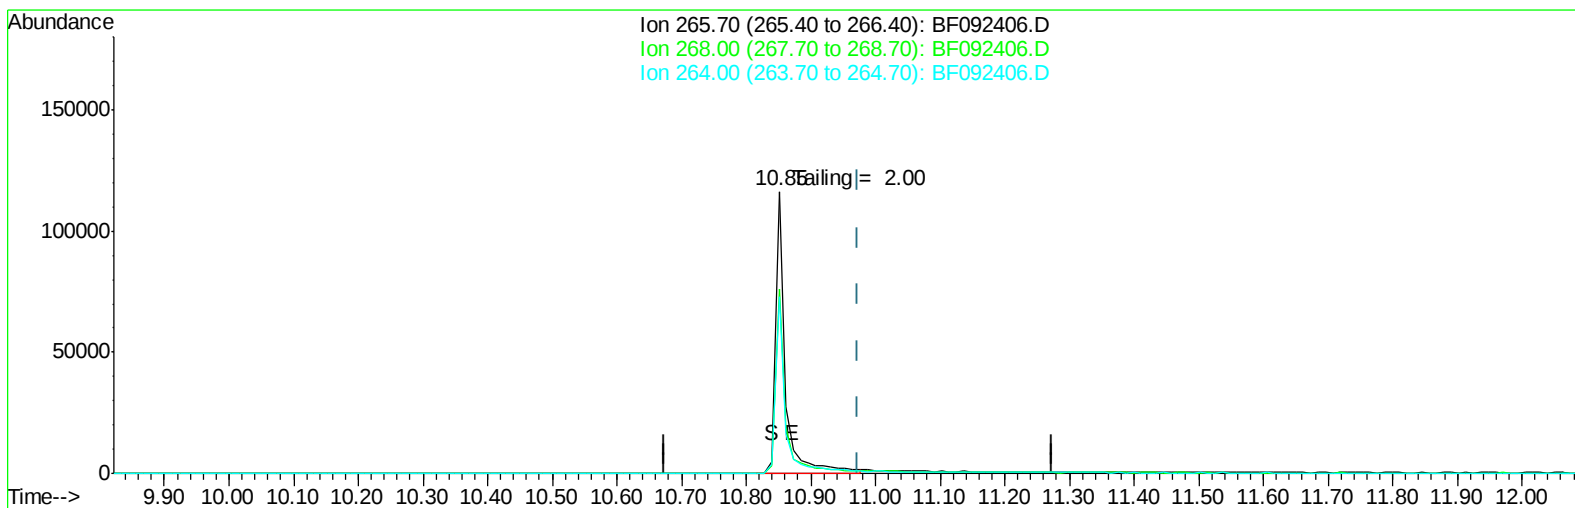

TIC: BF092406.D

(69) Pentachlorophenol (C)




10.850min (-0.123) 46123.66ng

response 133621

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.36
264.00	62.90	62.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF012117\
 Data File : BF092406.D
 Acq On : 21 Jan 2017 10:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 07:51:23 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 15:43:51 2017
 Response via : Initial Calibration

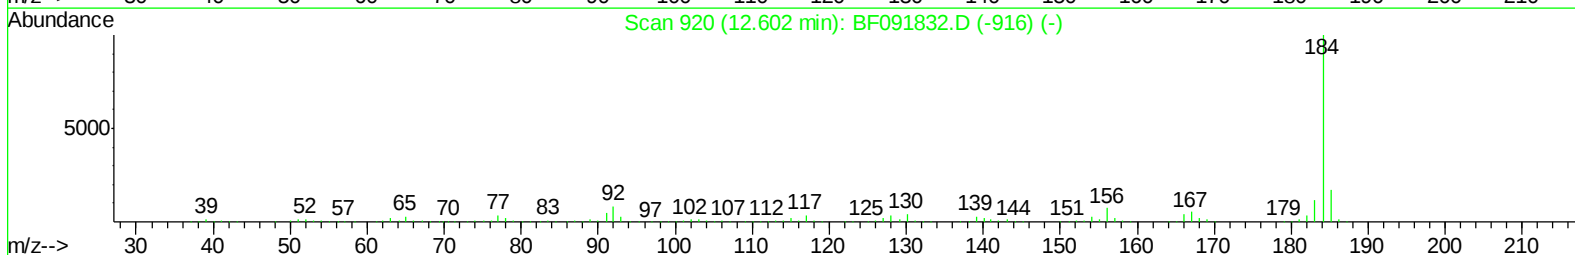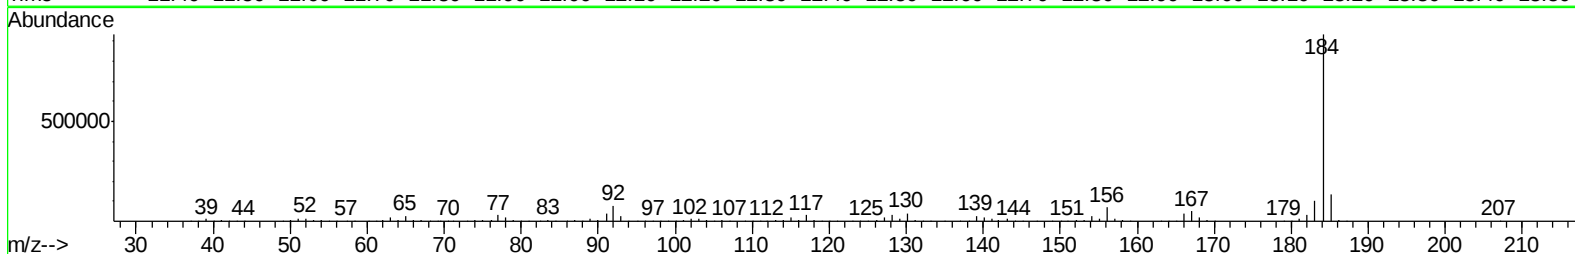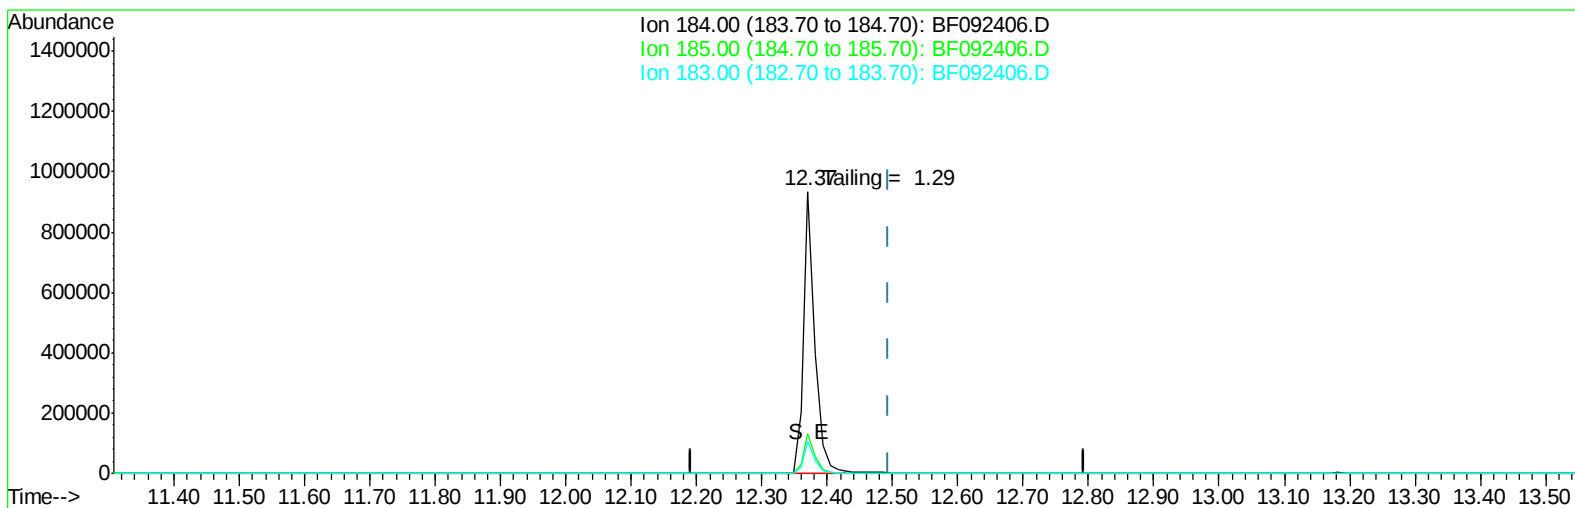

TIC: BF092406.D

(76) Benzidine

12.371min (-0.123) -20.00ng

response 1165953

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.26
183.00	11.50	11.26
0.00	0.00	0.00