

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012117\
 Data File : BF092413.D
 Acq On : 21 Jan 2017 15:22
 Operator : UM/SJ
 Sample : I1326-01RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-02-001-ARE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.597	258	259	271	rVB3	53824	104927	6.59%	1.011%
2	5.111	302	304	317	rBV	128780	277823	17.46%	2.678%
3	6.197	396	399	405	rBV	205402	301417	18.94%	2.905%
4	6.289	405	407	411	rVB	294823	331980	20.86%	3.199%
5	6.506	424	426	429	rBV	671398	710116	44.62%	6.844%
6	6.666	438	440	447	rVB	257008	245676	15.44%	2.368%
7	7.089	475	477	488	rVB	167478	189465	11.90%	1.826%
8	7.797	537	539	542	rBV	1020893	994644	62.49%	9.586%
9	8.883	631	634	636	rBV	503463	536689	33.72%	5.172%
10	9.283	668	669	672	rBV	43446	45549	2.86%	0.439%
11	9.546	689	692	694	rBV	1829951	1591626	100.00%	15.339%
12	10.335	759	761	771	rBV	256367	292001	18.35%	2.814%
13	11.021	819	821	824	rBV	1596248	1533361	96.34%	14.778%
14	12.449	944	946	949	rBV	62985	59961	3.77%	0.578%
15	12.609	957	960	962	rBV	505323	592967	37.26%	5.715%
16	13.158	1005	1008	1009	rBV	26374	37291	2.34%	0.359%
17	13.649	1049	1051	1054	rBV	1406583	1370485	86.11%	13.208%
18	14.998	1166	1169	1172	rBV	895707	1076613	67.64%	10.376%
19	15.387	1200	1203	1206	rBV	26438	40186	2.52%	0.387%
20	15.787	1235	1238	1240	rVB	25483	43254	2.72%	0.417%


Sum of corrected areas: 10376031

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012117\
Data File : BF092413.D
Acq On : 21 Jan 2017 15:22
Operator : UM/SJ
Sample : I1326-01RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-001-ARE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

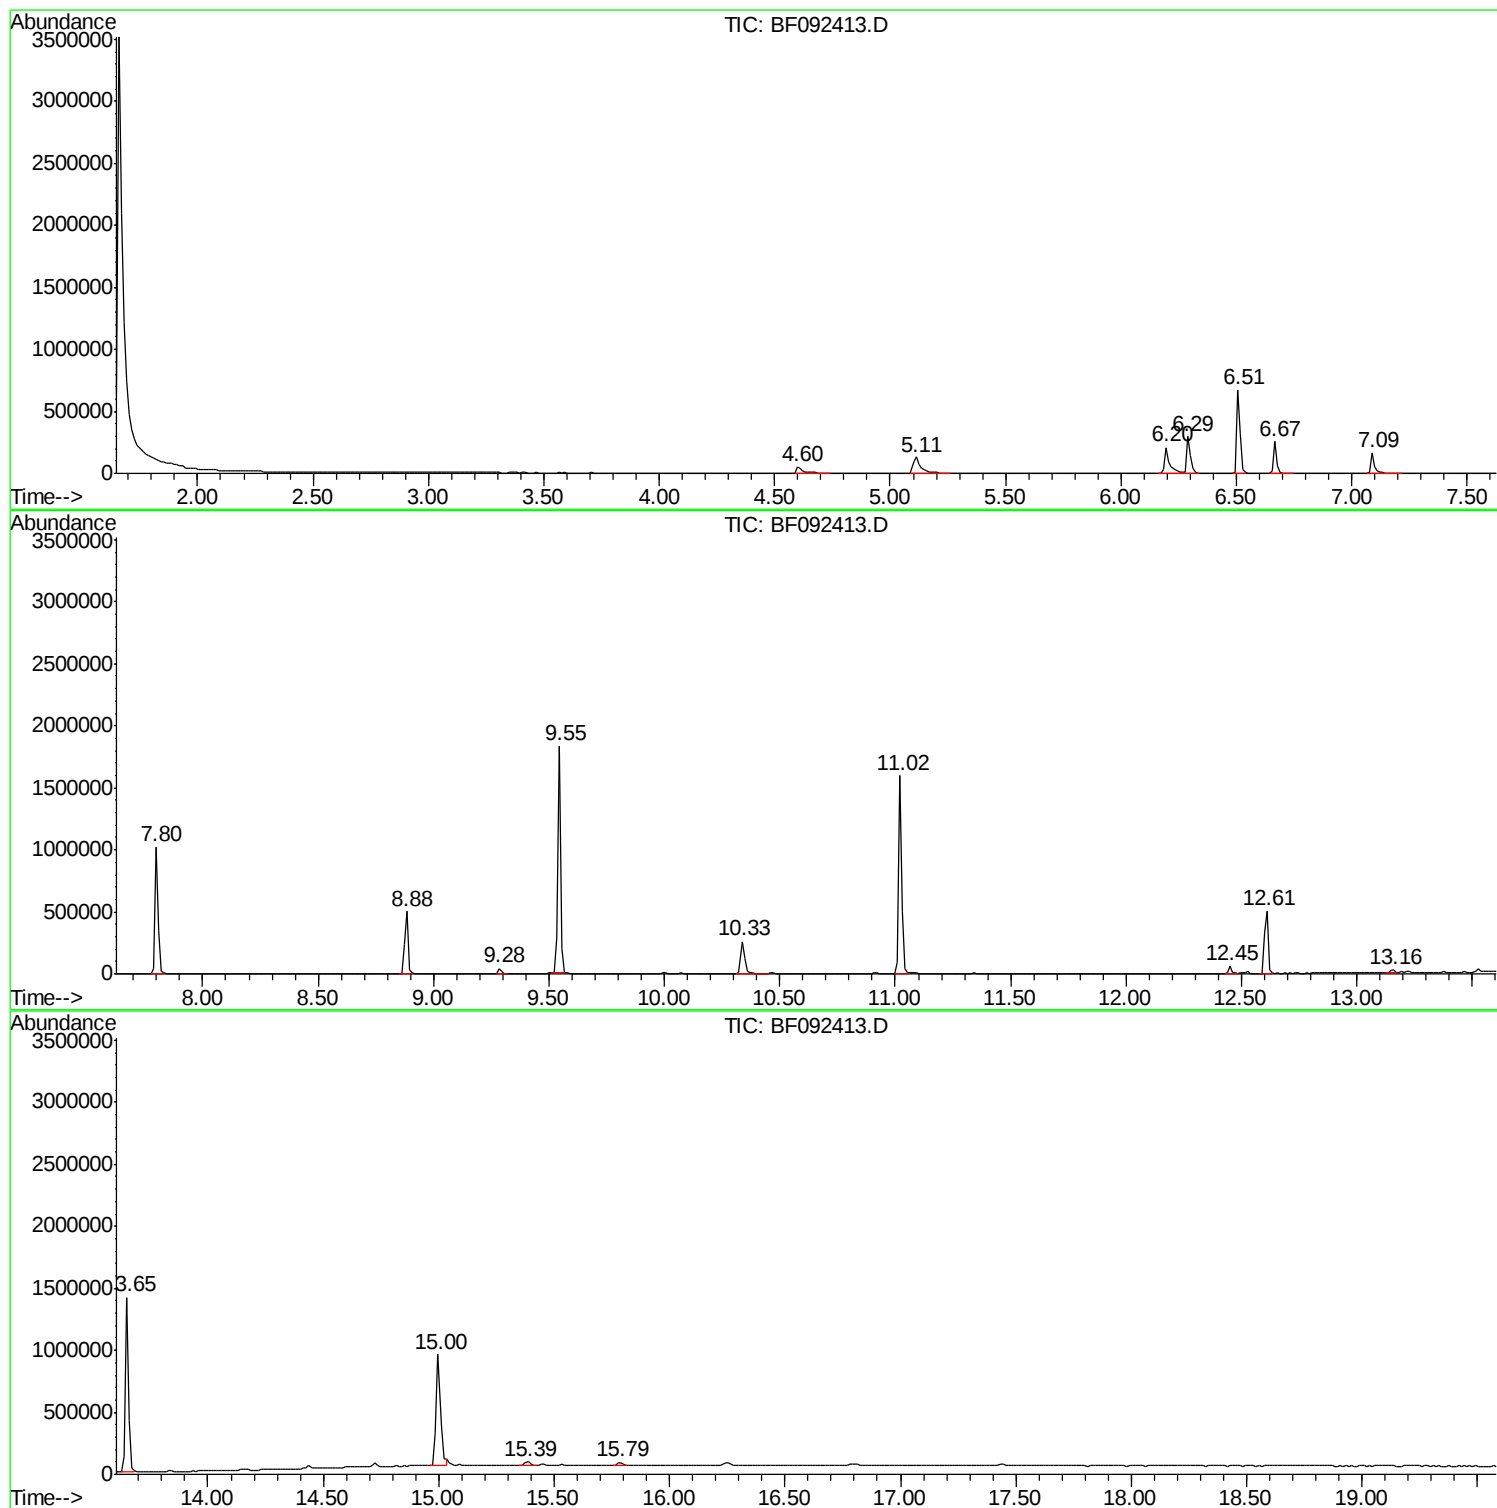

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF012117\
Data_File : BF092413.D
Acq_On : 21-Jan-2017 15:222
Operator : UM/SJJ
Sample : I1326-01REE
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-001-ARE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
