


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012117\
 Data File : BF092406.D
 Acq On : 21 Jan 2017 10:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

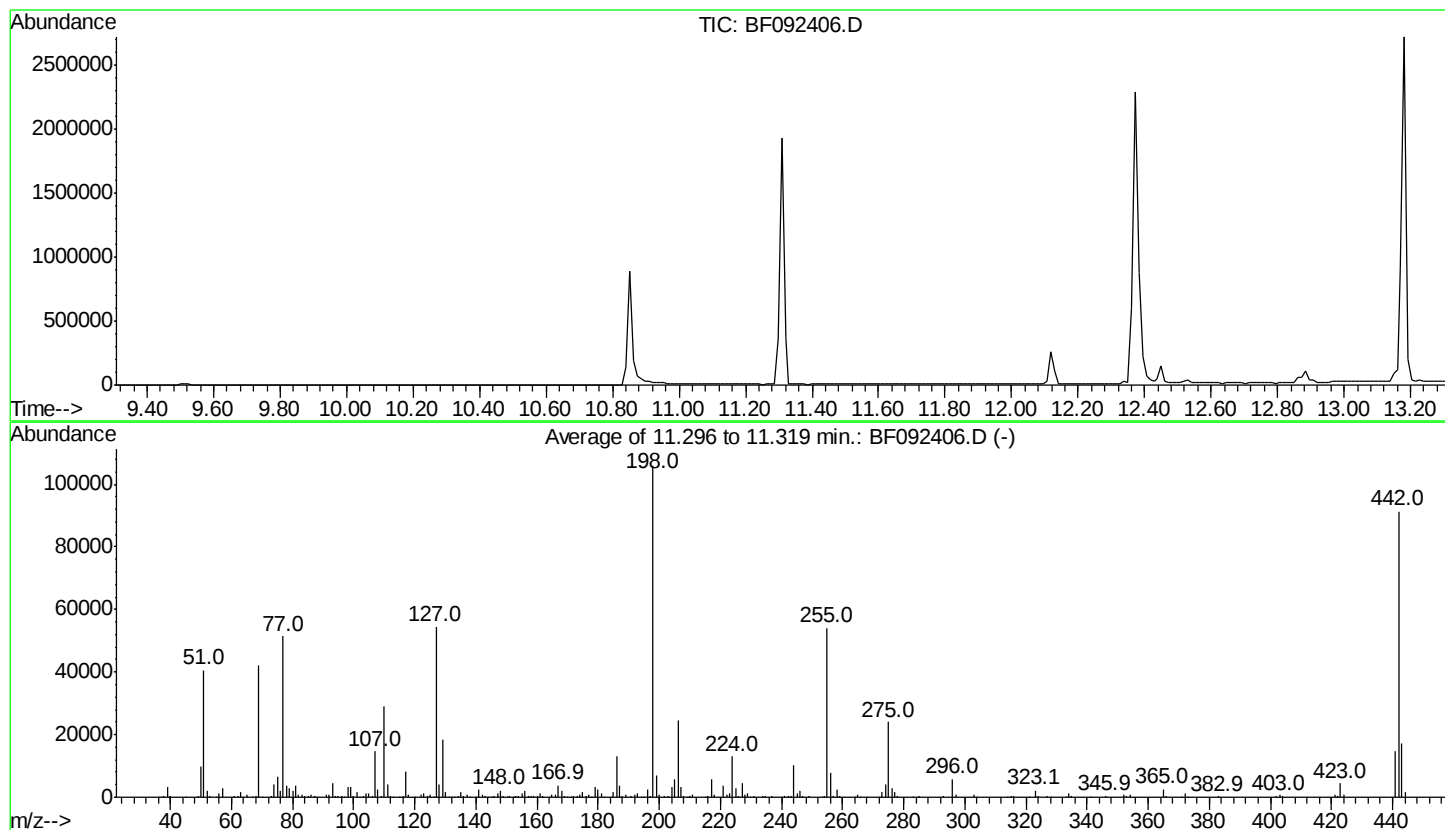

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	40613	PASS
68	69	0.00	2	1.5	625	PASS
69	198	0.00	100	39.9	42261	PASS
70	69	0.00	2	0.4	179	PASS
127	198	10	80	51.4	54500	PASS
197	198	0.00	2	0.5	502	PASS
198	198	100	100	100.0	105944	PASS
199	198	5	9	6.7	7075	PASS
275	198	10	60	22.6	23941	PASS
365	198	1	100	2.5	2613	PASS
441	442	0.01	24	15.9	14541	PASS
442	198	50	100	86.3	91389	PASS
443	442	15	24	19.0	17338	PASS