
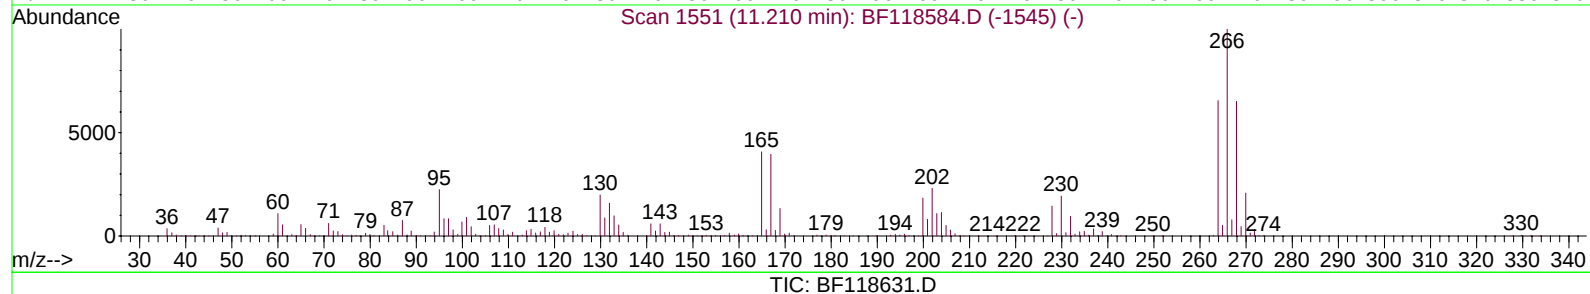
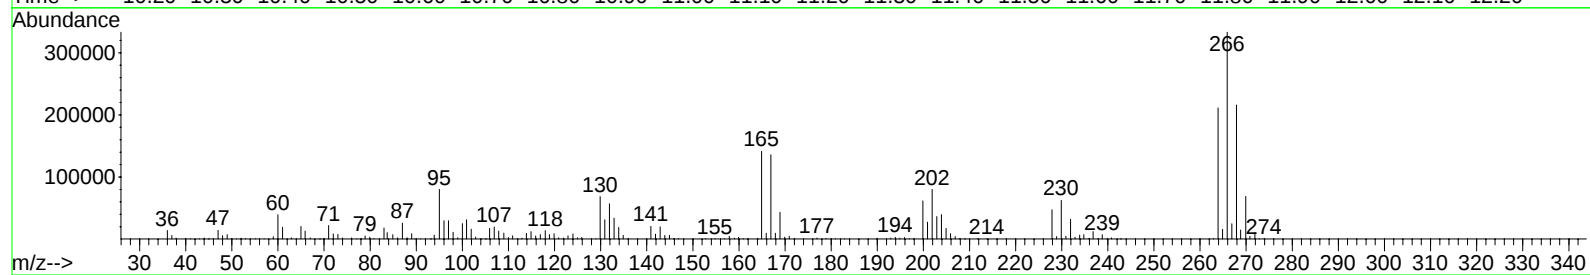


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012120\
Data File : BF118631.D
Acq On : 21 Jan 2020 12:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 18:02:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 20 14:45:03 2020
Response via : Initial Calibration

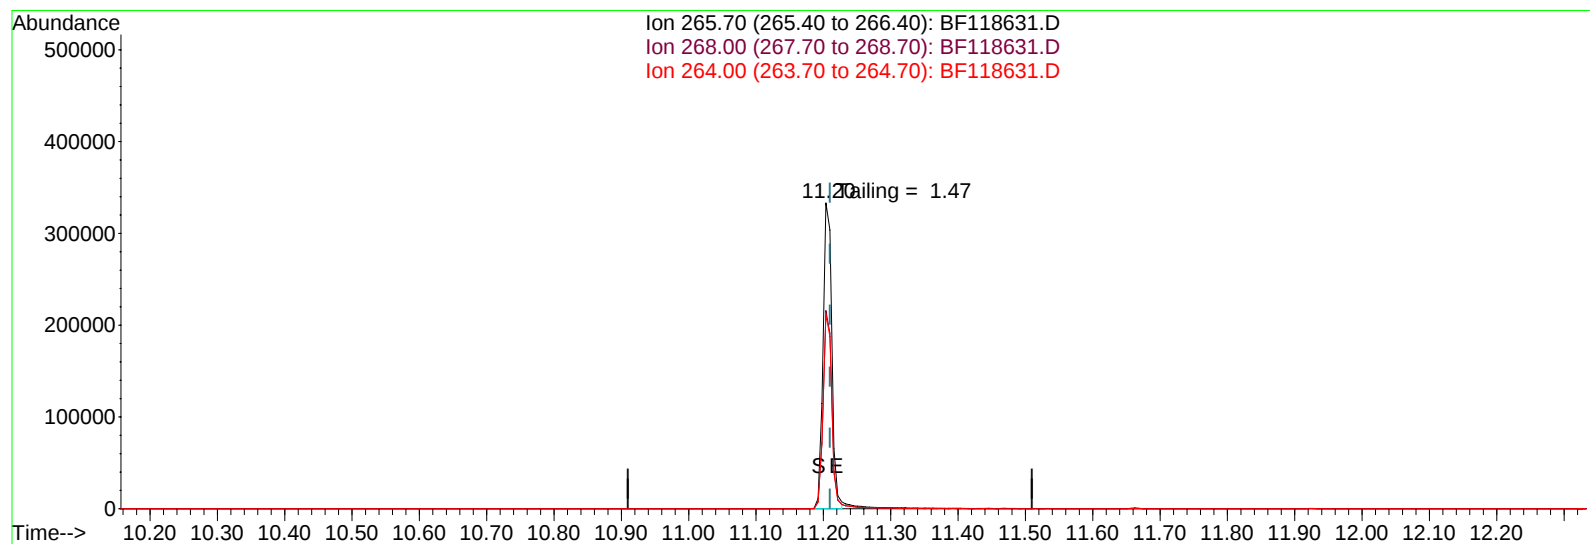

(70) Pentachlorophenol (C)




11.204min (-0.006) 30166.87ng

response 312220

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	64.78
264.00	65.50	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012120\
 Data File : BF118631.D
 Acq On : 21 Jan 2020 12:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 18:02:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 20 14:45:03 2020
 Response via : Initial Calibration

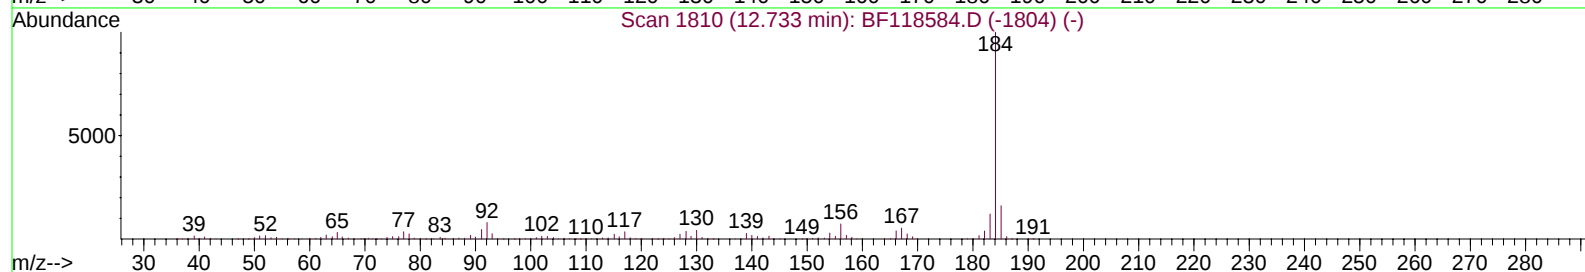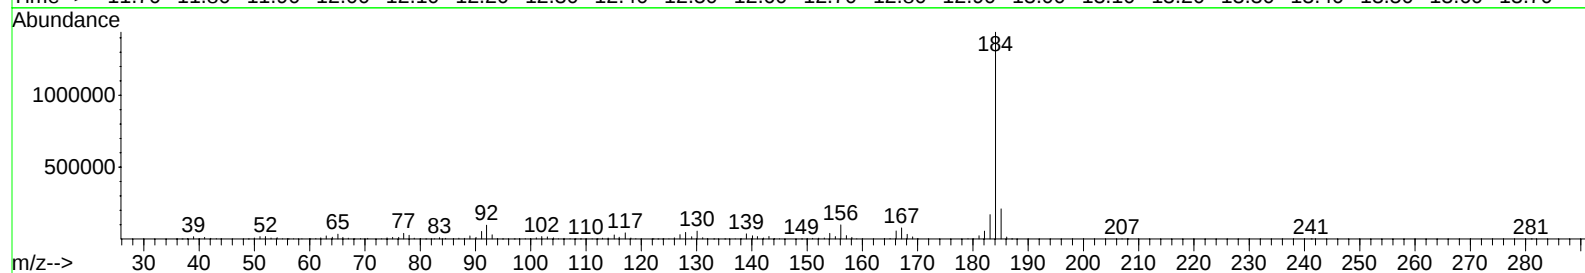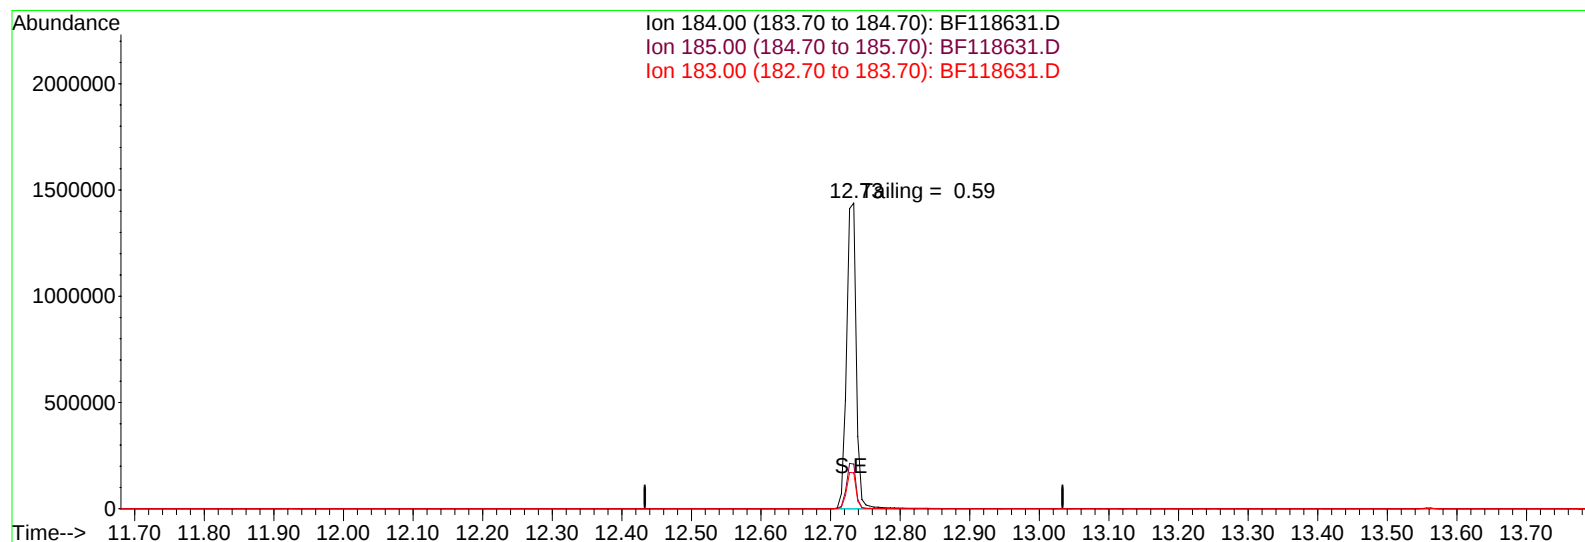

TIC: BF118631.D

(77) Benzidine

12.733min (-12.733) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	16.10	0.00#
183.00	12.00	0.00#
0.00	0.00	0.00