


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012120\
 Data File : BF118631.D
 Acq On : 21 Jan 2020 12:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 20 14:45:03 2020

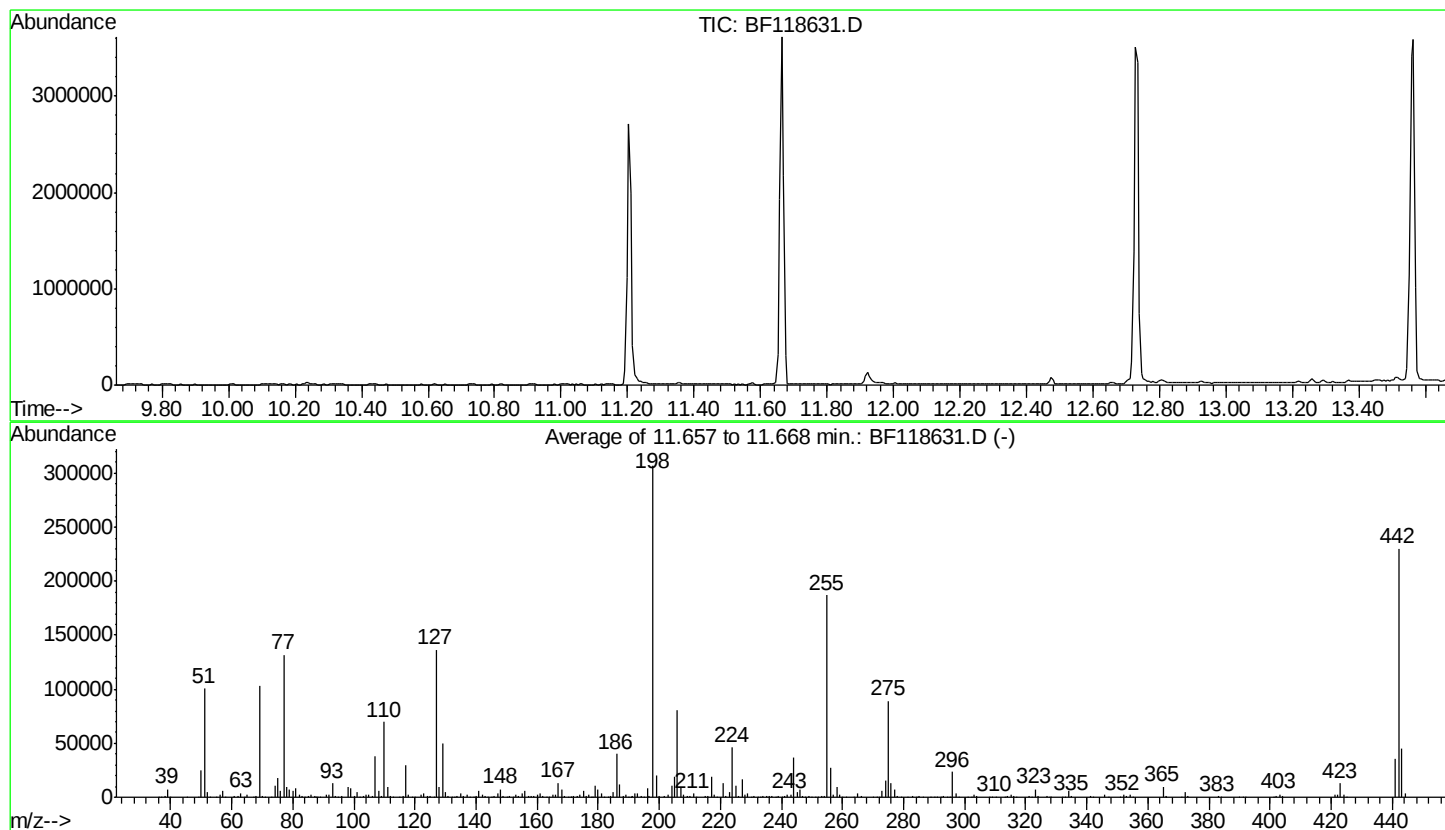

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	100448	PASS
68	69	0.00	2	1.7	1796	PASS
69	198	0.00	100	33.7	103515	PASS
70	69	0.00	2	0.6	651	PASS
127	198	10	80	44.5	136720	PASS
197	198	0.00	2	0.5	1579	PASS
198	198	100	100	100.0	307008	PASS
199	198	5	9	6.6	20377	PASS
275	198	10	60	29.0	89122	PASS
365	198	1	100	3.3	10068	PASS
441	198	0.01	100	11.6	35540	PASS
442	198	50	100	75.0	230272	PASS
443	442	15	24	19.7	45333	PASS