


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012120\
 Data File : BF118656.D
 Acq On : 22 Jan 2020 9:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 20 14:45:03 2020

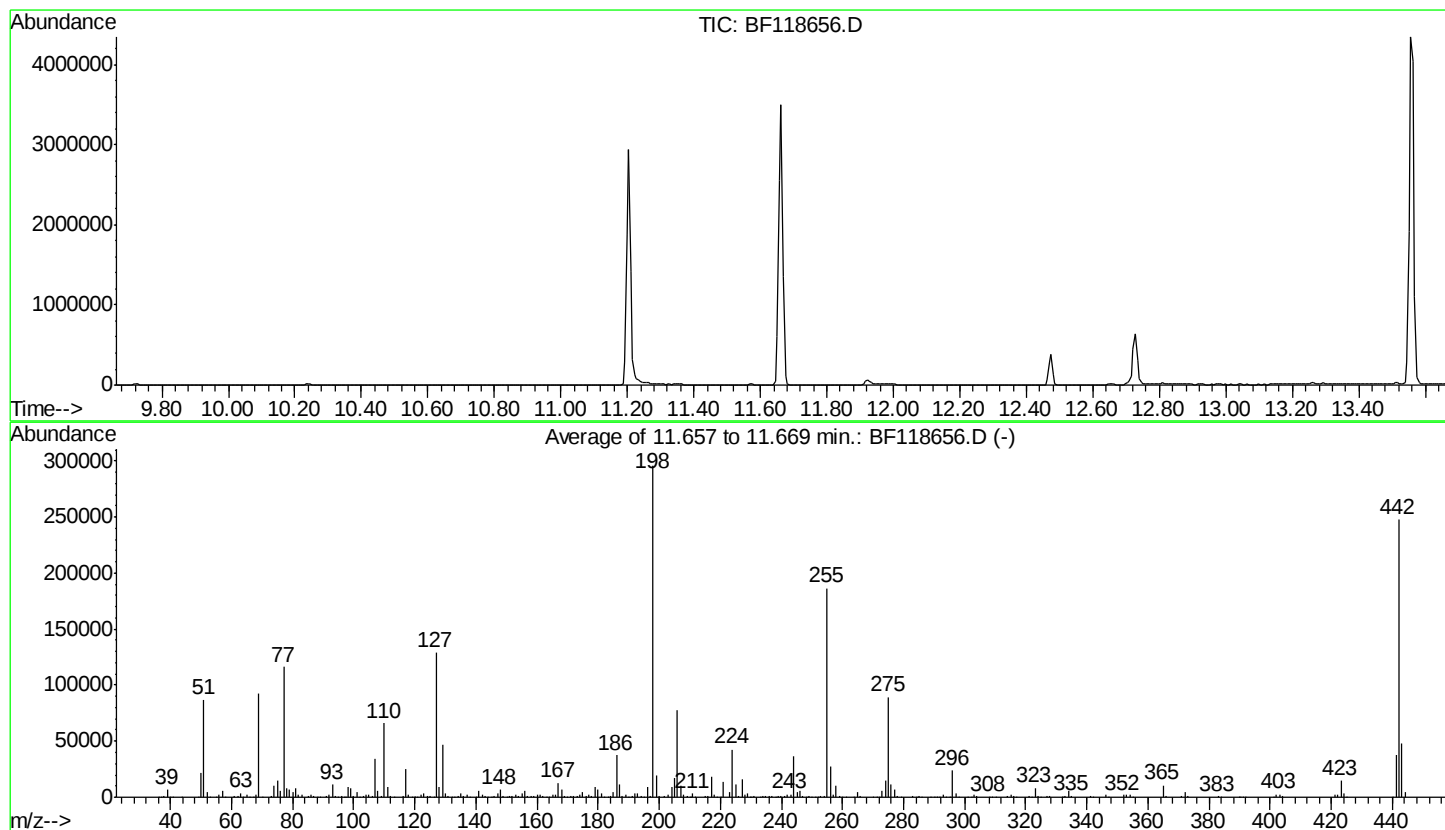

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	87269	PASS
68	69	0.00	2	2.0	1842	PASS
69	198	0.00	100	31.4	92813	PASS
70	69	0.00	2	0.5	451	PASS
127	198	10	80	43.5	128618	PASS
197	198	0.00	2	0.4	1324	PASS
198	198	100	100	100.0	295872	PASS
199	198	5	9	6.8	19985	PASS
275	198	10	60	30.1	89189	PASS
365	198	1	100	3.6	10529	PASS
441	198	0.01	100	12.8	37842	PASS
442	198	50	100	83.7	247786	PASS
443	442	15	24	19.3	47858	PASS