
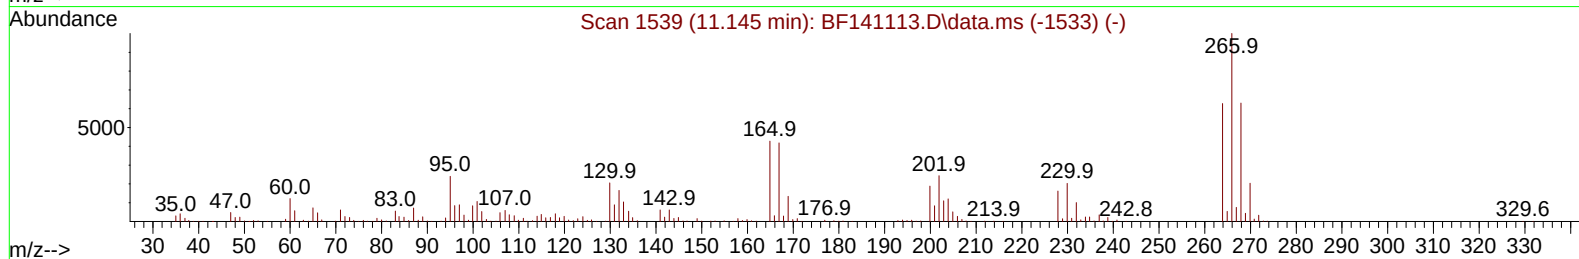
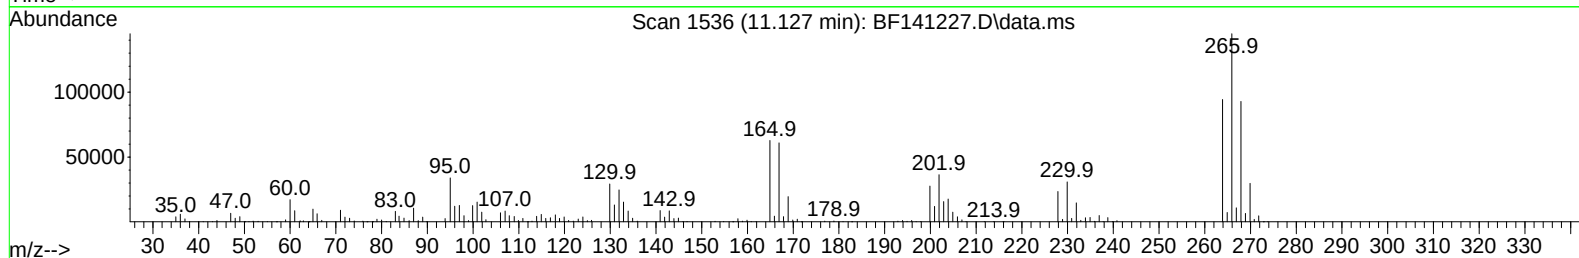


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012125\
Data File : BF141227.D
Acq On : 21 Jan 2025 11:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 13:04:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

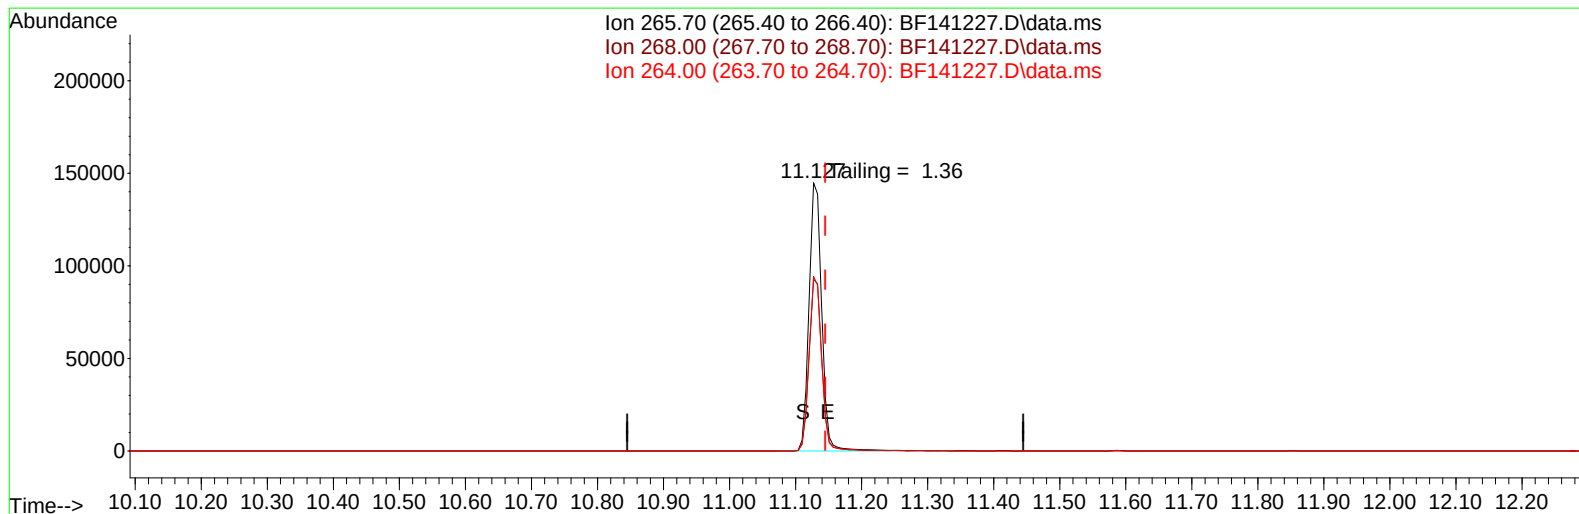

TIC: BF141227.D\data.ms

(70) Pentachlorophenol (C)




11.127min (-0.018) 406412.80 ng

response 193466

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.08
264.00	62.70	65.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012125\
Data File : BF141227.D
Acq On : 21 Jan 2025 11:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 13:04:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

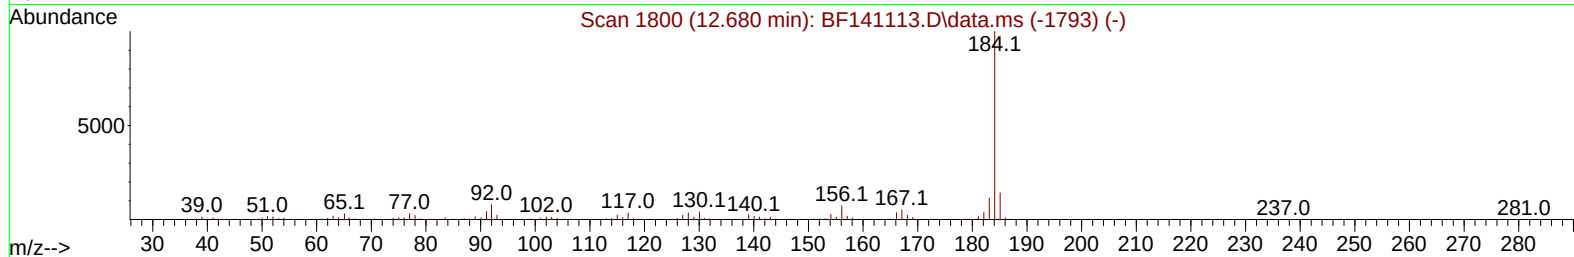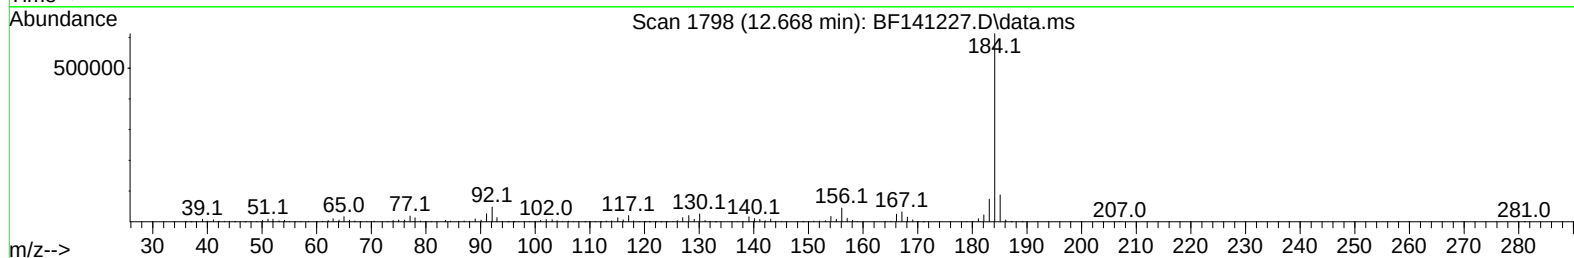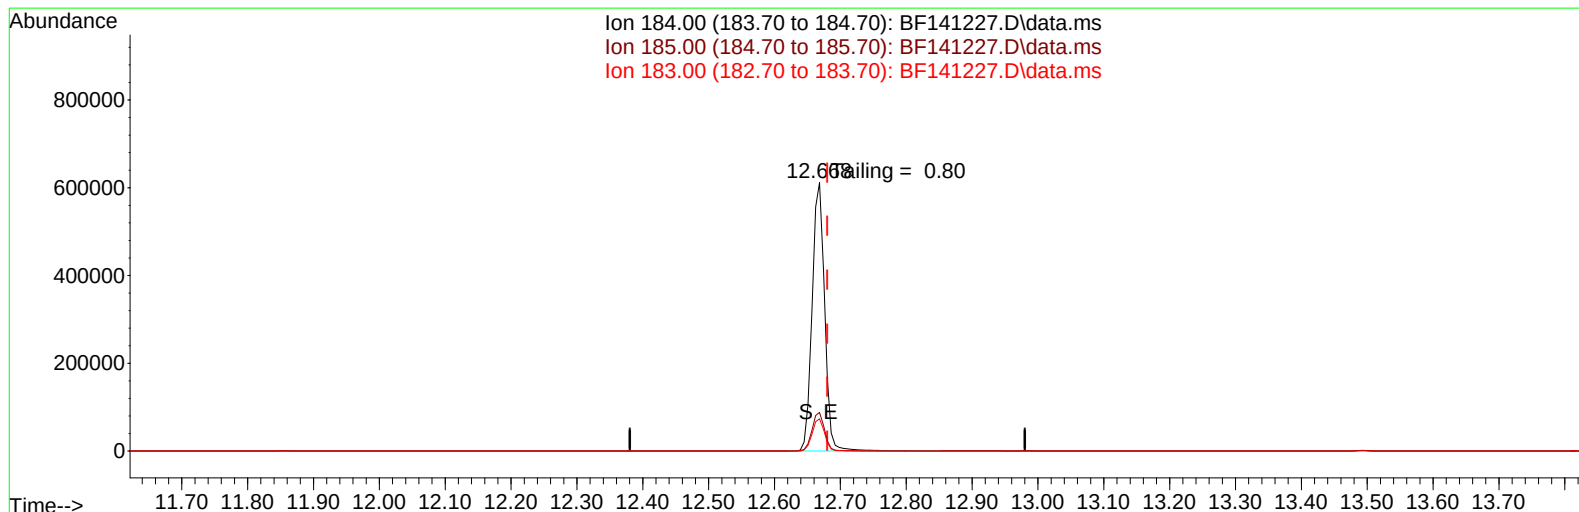

TIC: BF141227.D\data.ms

(77) Benzidine**12.668min (-0.012) 338150.89 ng****response 808933**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.36
183.00	11.50	11.99
0.00	0.00	0.00