
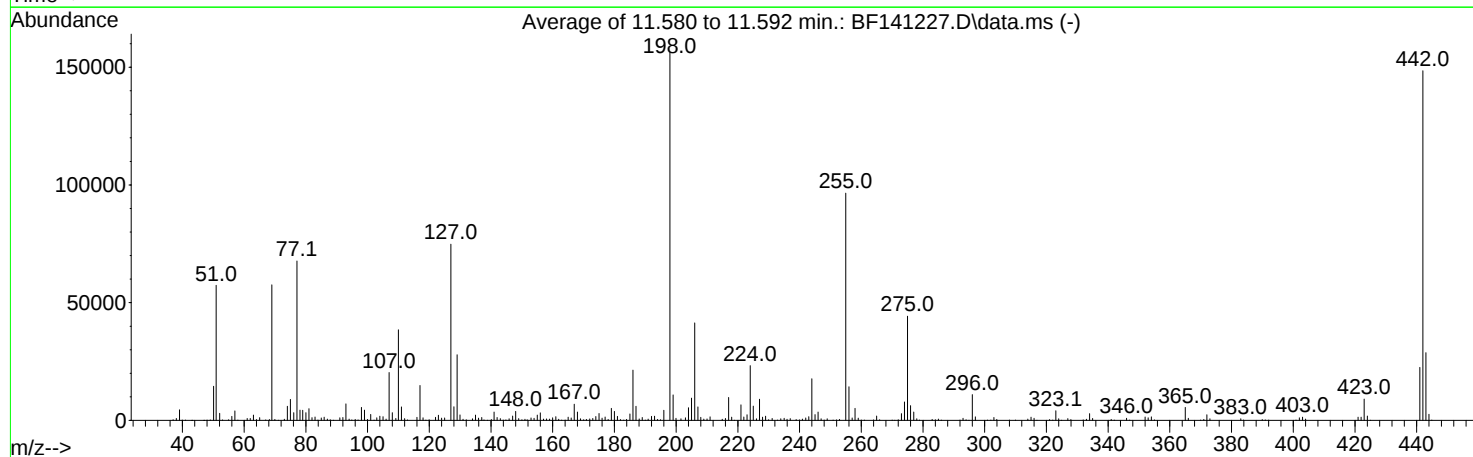


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012125\
Data File : BF141227.D
Acq On : 21 Jan 2025 11:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

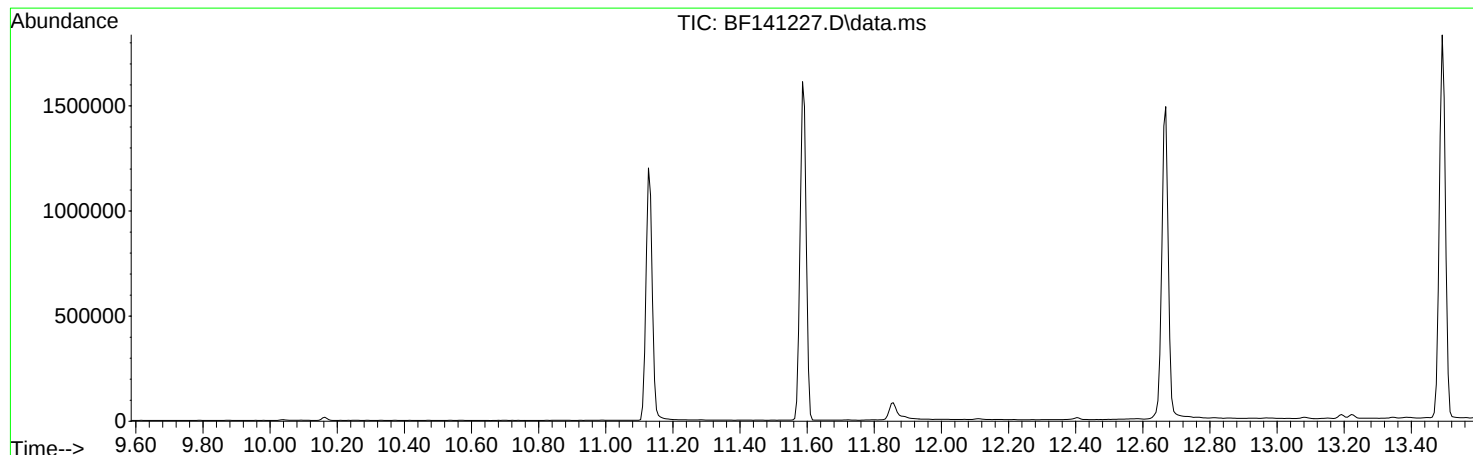




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	57342	PASS
68	69	0.00	2	0.6	339	PASS
69	198	0.00	100	36.8	57581	PASS
70	69	0.00	2	0.7	401	PASS
127	198	10	80	47.9	74851	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	156259	PASS
199	198	5	9	6.9	10802	PASS
275	198	10	60	28.3	44285	PASS
365	198	1	100	3.5	5484	PASS
441	198	0.01	100	14.4	22517	PASS
442	442	50	100	100.0	148496	PASS
443	442	15	24	19.4	28789	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012125\
Data File : BF141227.D
Acq On : 21 Jan 2025 11:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 21 13:04:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

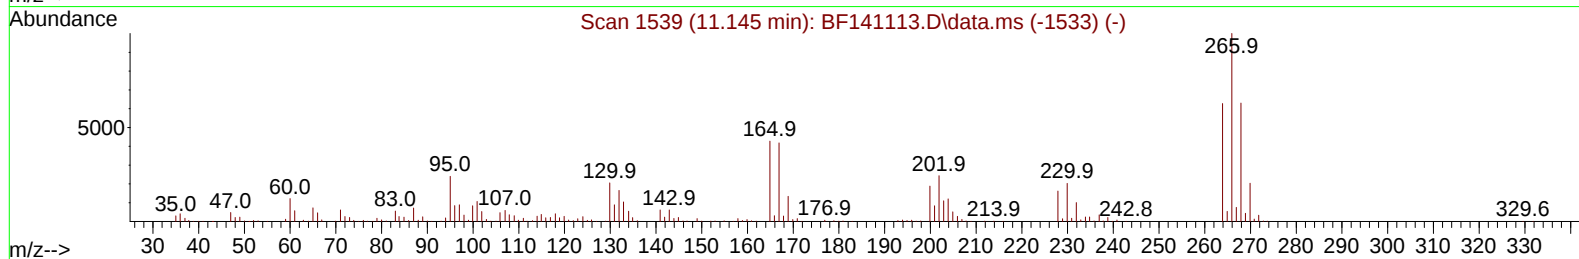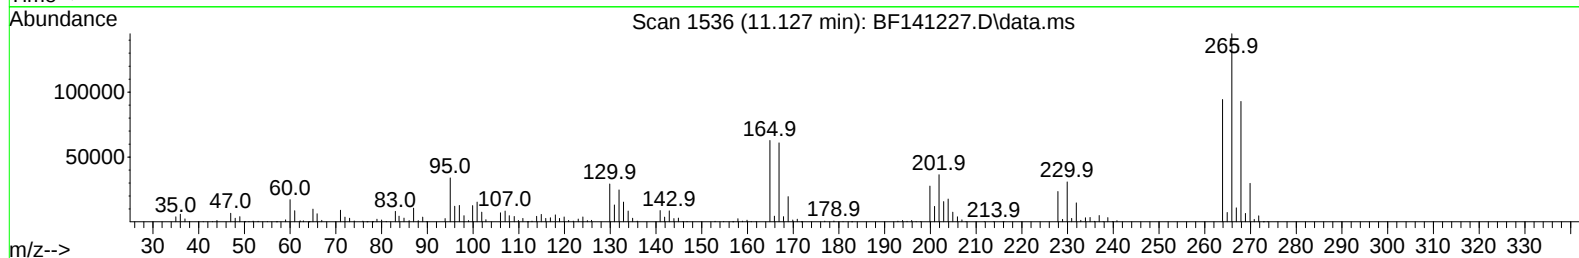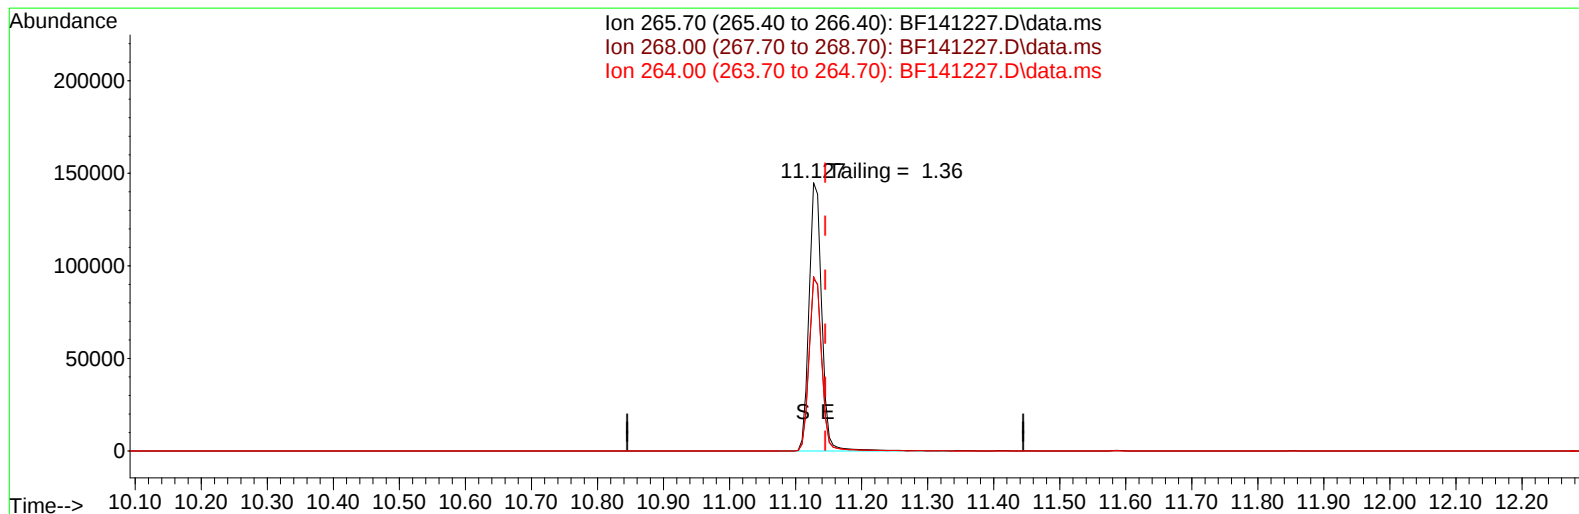

TIC: BF141227.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.018) 406412.80 ng




response 193466

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.08
264.00	62.70	65.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012125\
Data File : BF141227.D
Acq On : 21 Jan 2025 11:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 21 13:04:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

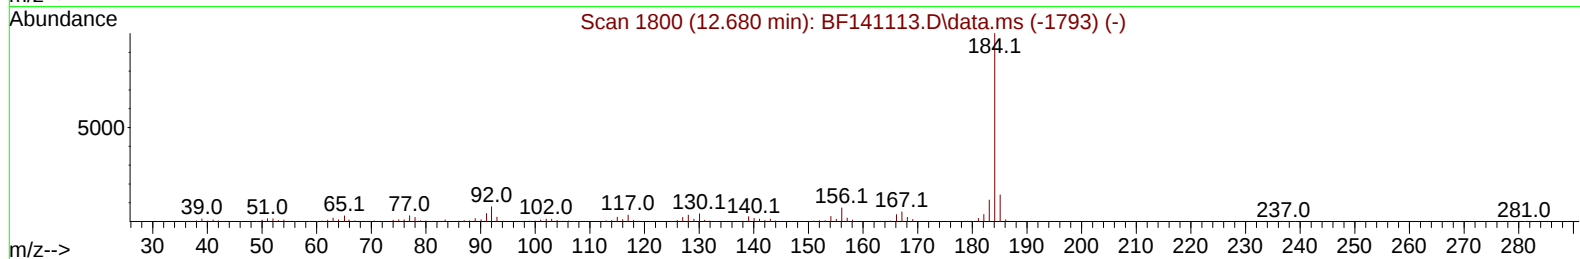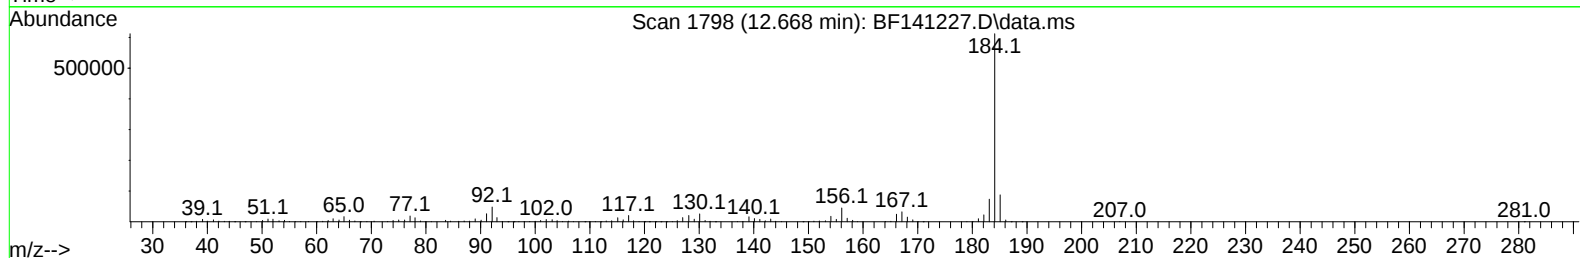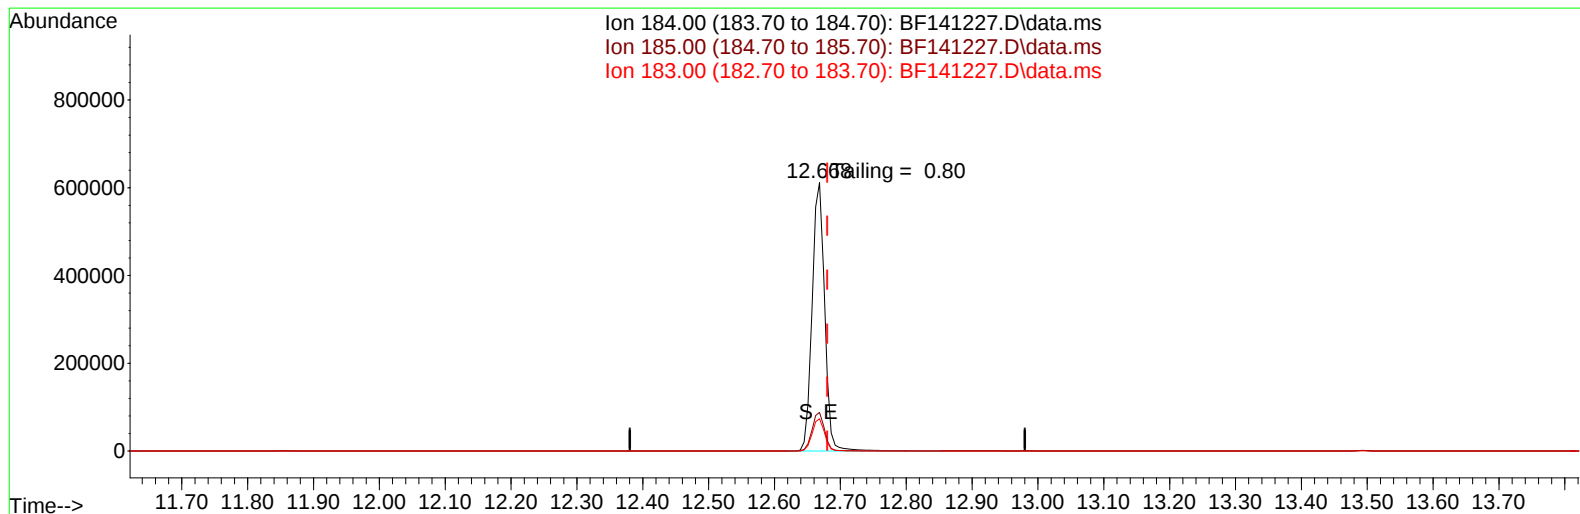

TIC: BF141227.D\data.ms

(77) Benzidine

12.668min (-0.012) 338150.89 ng

response 808933

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.36
183.00	11.50	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/21/2025	BNA_F	<u>BF141227.D</u>
Compound Name	Response	Retention Time
DDT	453150	13.492
DDD	10240	13.192
DDE	268	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10508	463658	2.27

Instrument :
BNA_F
ClientSampleId :
DFTPP