


Data Path : Z:\HPCHEM1\BNA F\Data\BF012215\
 Data File : BF077024.D
 Acq On : 22 Jan 2015 23:26
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 21 14:45:53 2015

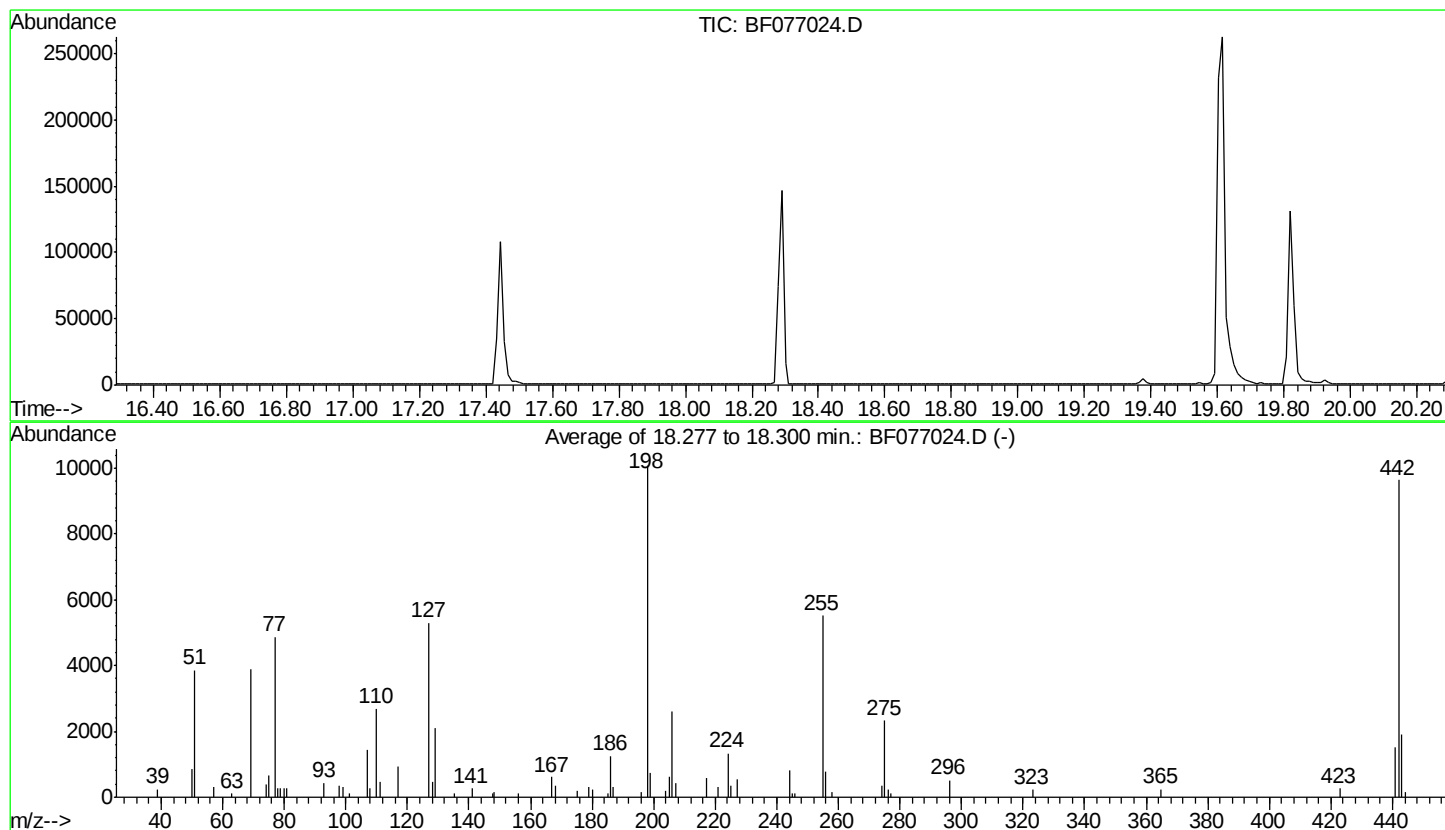

AutoFind: Scans 1504, 1505, 1506; Background Corrected with Scan 1501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	3867	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.6	3890	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	5305	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10073	PASS
199	198	5	9	7.4	750	PASS
275	198	10	60	23.0	2319	PASS
365	198	1	100	2.3	235	PASS
441	442	0.01	24	15.6	1506	PASS
442	198	50	100	95.7	9639	PASS
443	442	15	24	19.8	1910	PASS