


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012216\
 Data File : BF084583.D
 Acq On : 22 Jan 2016 10:18
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 14 14:15:52 2016

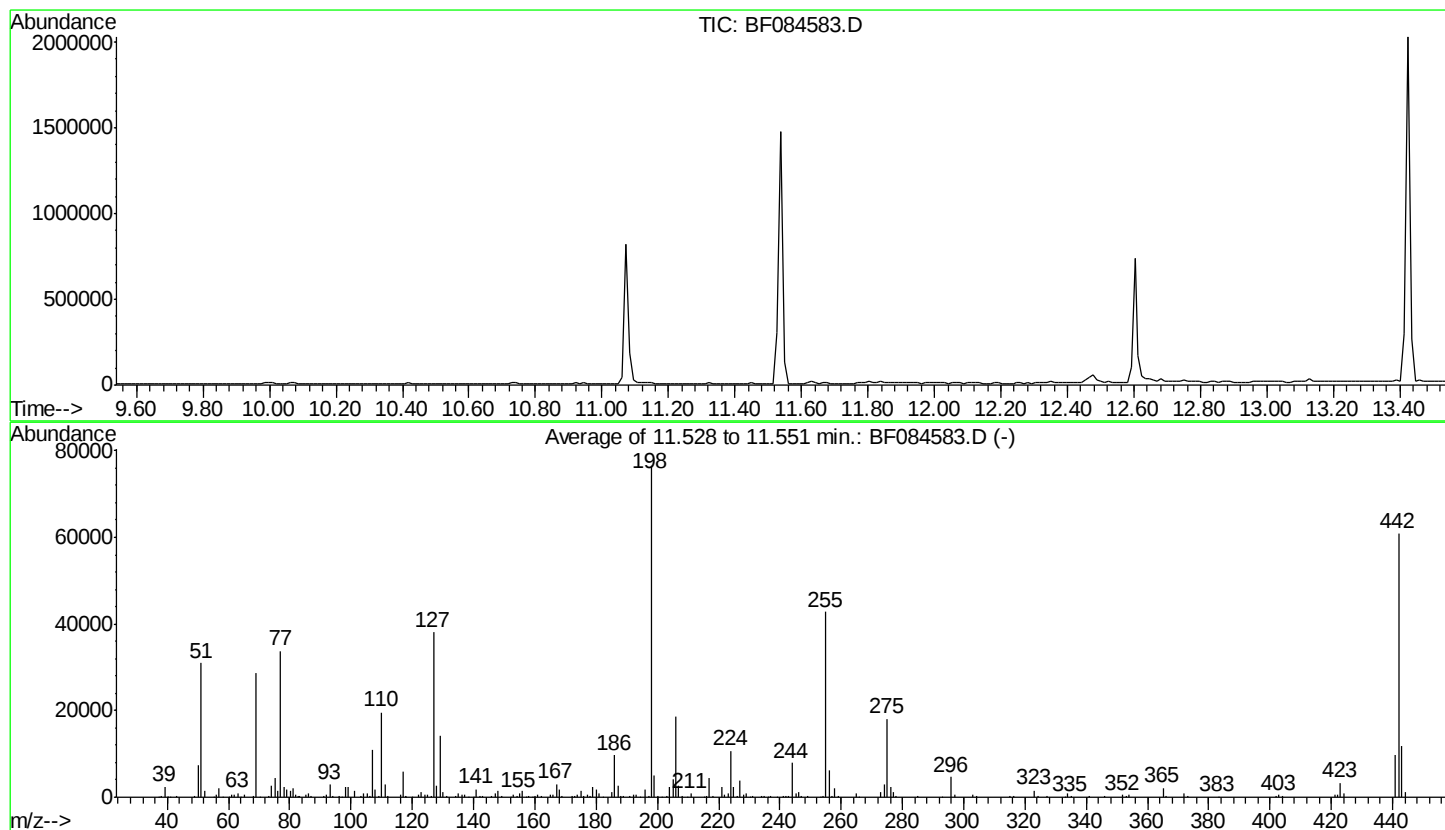

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	30897	PASS
68	69	0.00	2	1.3	377	PASS
69	198	0.00	100	37.3	28577	PASS
70	69	0.00	2	0.4	109	PASS
127	198	10	80	49.7	38059	PASS
197	198	0.00	2	0.5	370	PASS
198	198	100	100	100.0	76549	PASS
199	198	5	9	6.6	5015	PASS
275	198	10	60	23.6	18079	PASS
365	198	1	100	2.8	2137	PASS
441	442	0.01	24	16.1	9804	PASS
442	198	50	100	79.5	60821	PASS
443	442	15	24	19.6	11895	PASS