


Data Path : Z:\HPCHEM1\BNA F\Data\BF012218\
Data File : BF102287.D
Acq On : 22 Jan 2018 9:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 23 00:43:41 2018

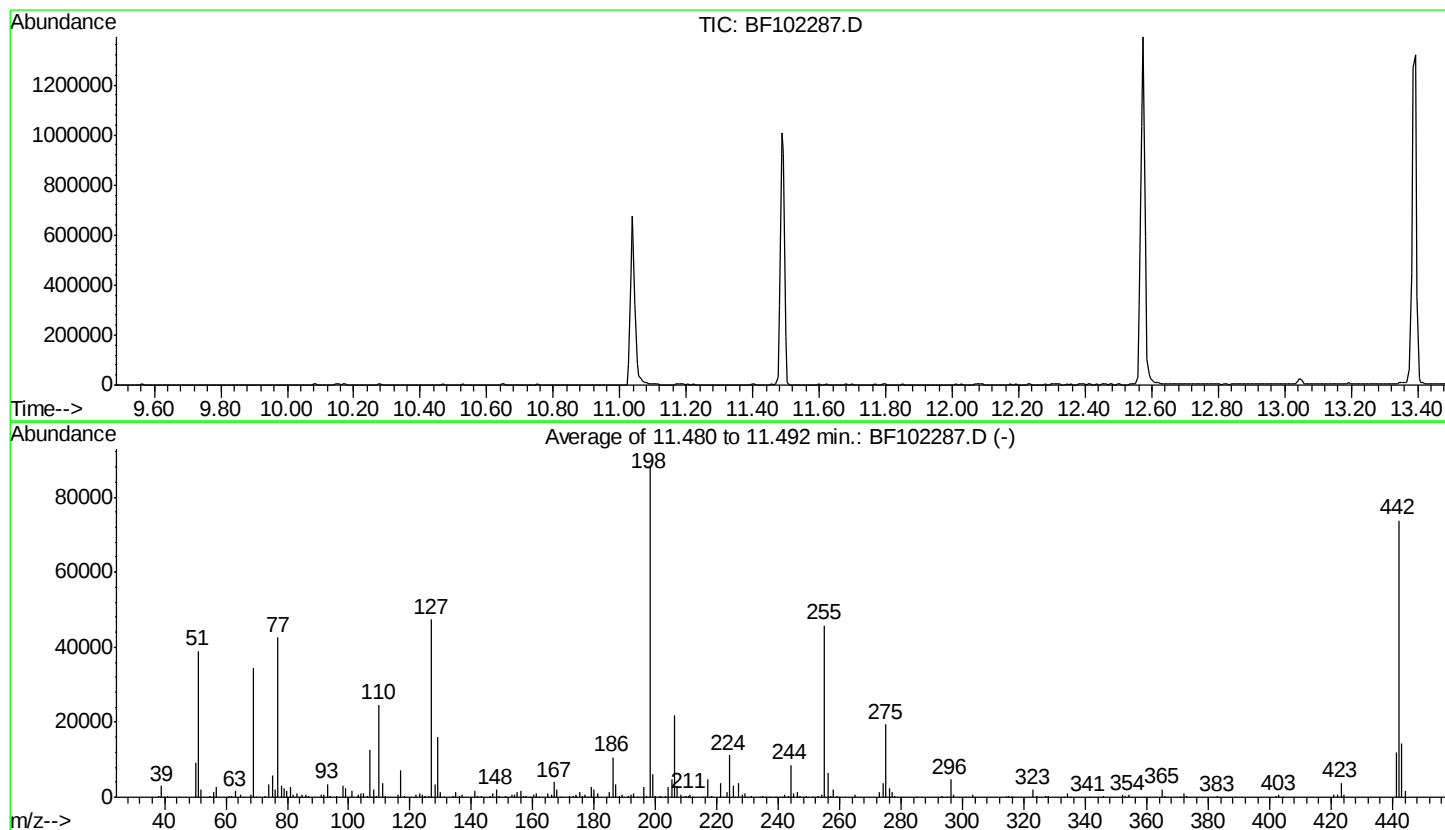

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	39037	PASS
68	69	0.00	2	1.9	642	PASS
69	198	0.00	100	38.8	34330	PASS
70	69	0.00	2	0.3	110	PASS
127	198	10	80	53.6	47352	PASS
197	198	0.00	2	0.5	421	PASS
198	198	100	100	100.0	88378	PASS
199	198	5	9	6.9	6075	PASS
275	198	10	60	21.9	19373	PASS
365	198	1	100	2.3	2069	PASS
441	443	0.01	100	83.1	11853	PASS
442	198	50	100	83.6	73857	PASS
443	442	15	24	19.3	14270	PASS