


Data Path : Z:\HPCHEM1\BNA F\Data\BF012218\
 Data File : BF102296.D
 Acq On : 22 Jan 2018 13:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 23 00:43:41 2018

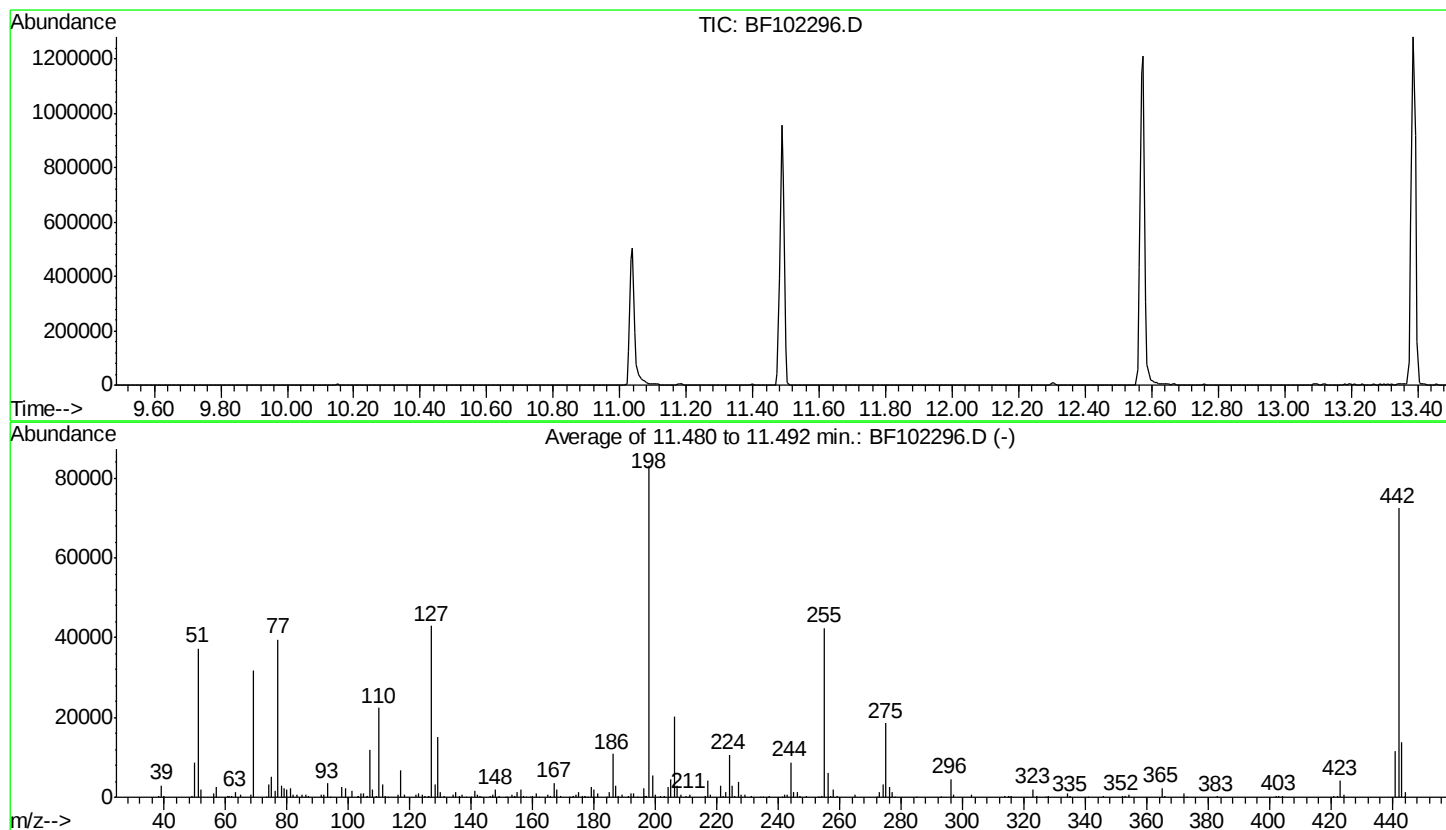

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	37269	PASS
68	69	0.00	2	1.8	573	PASS
69	198	0.00	100	38.4	31930	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.6	42869	PASS
197	198	0.00	2	0.6	486	PASS
198	198	100	100	100.0	83141	PASS
199	198	5	9	6.7	5591	PASS
275	198	10	60	22.3	18558	PASS
365	198	1	100	2.8	2319	PASS
441	443	0.01	100	83.4	11522	PASS
442	198	50	100	87.1	72413	PASS
443	442	15	24	19.1	13814	PASS