


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012218\
Data File : BF102323.D
Acq On : 23 Jan 2018 2:59
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 23 00:43:41 2018

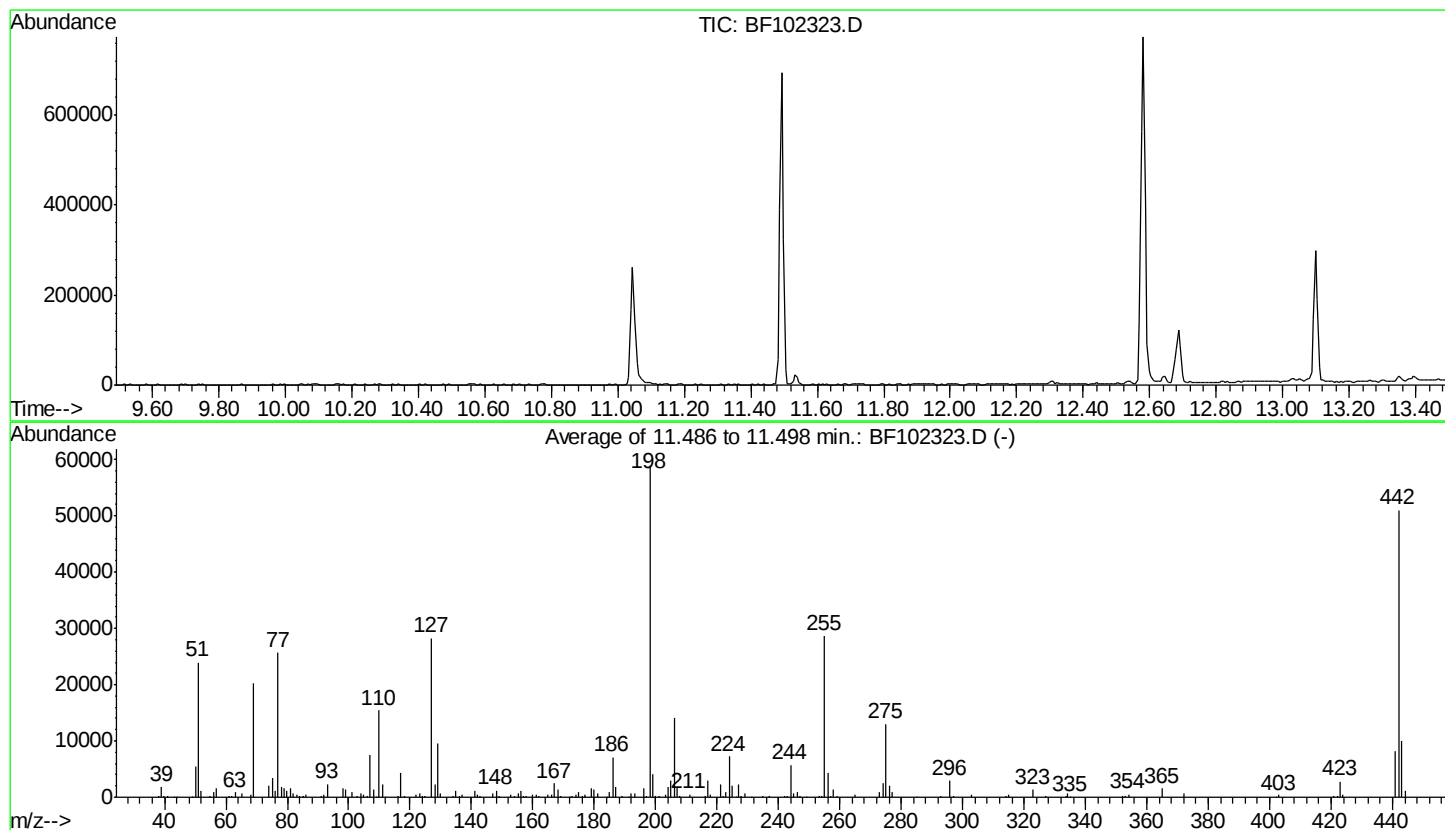

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	23957	PASS
68	69	0.00	2	1.8	373	PASS
69	198	0.00	100	34.5	20342	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	28247	PASS
197	198	0.00	2	0.3	186	PASS
198	198	100	100	100.0	58920	PASS
199	198	5	9	6.8	3990	PASS
275	198	10	60	22.2	13058	PASS
365	198	1	100	2.6	1517	PASS
441	443	0.01	100	82.9	8237	PASS
442	198	50	100	86.6	51034	PASS
443	442	15	24	19.5	9938	PASS