
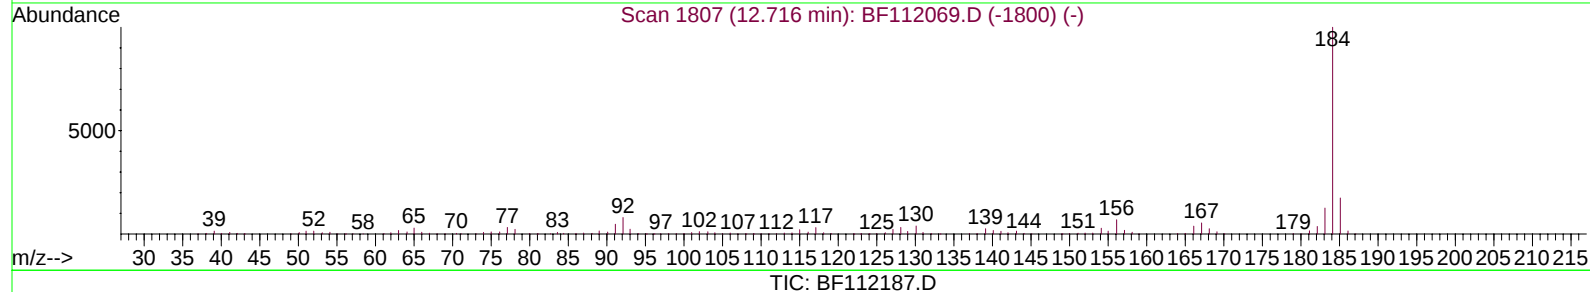
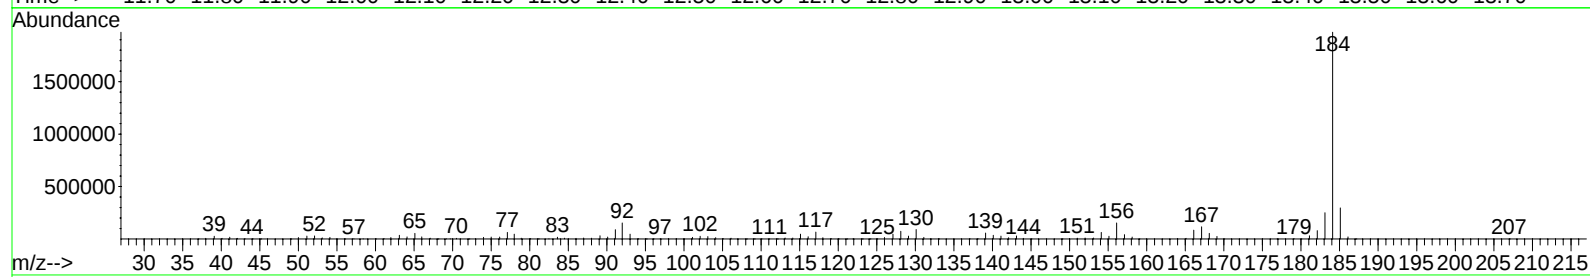


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012219\
 Data File : BF112187.D
 Acq On : 22 Jan 2019 12:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 17:48:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 19 01:02:12 2019
 Response via : Initial Calibration

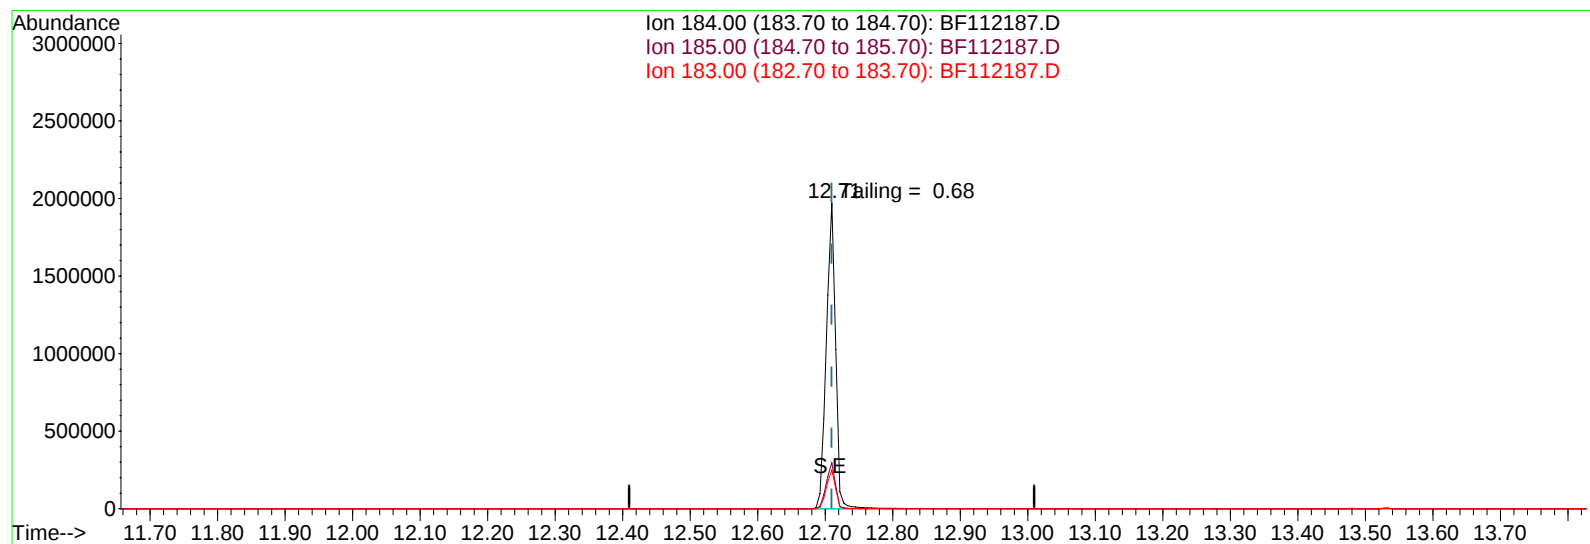

(77) Benzidine




12.710min (+0.000) 98332.14ng

response 1873371

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	15.07
183.00	12.50	12.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012219\
Data File : BF112187.D
Acq On : 22 Jan 2019 12:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 17:48:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 19 01:02:12 2019
Response via : Initial Calibration

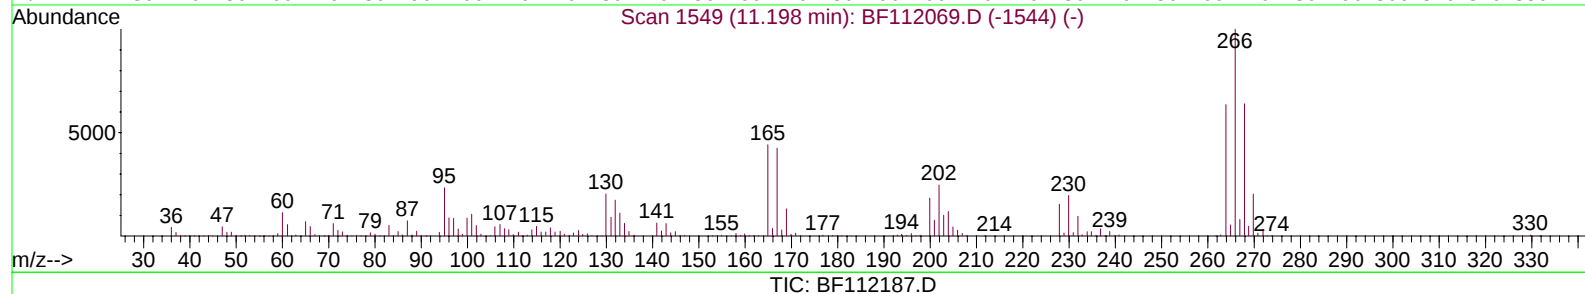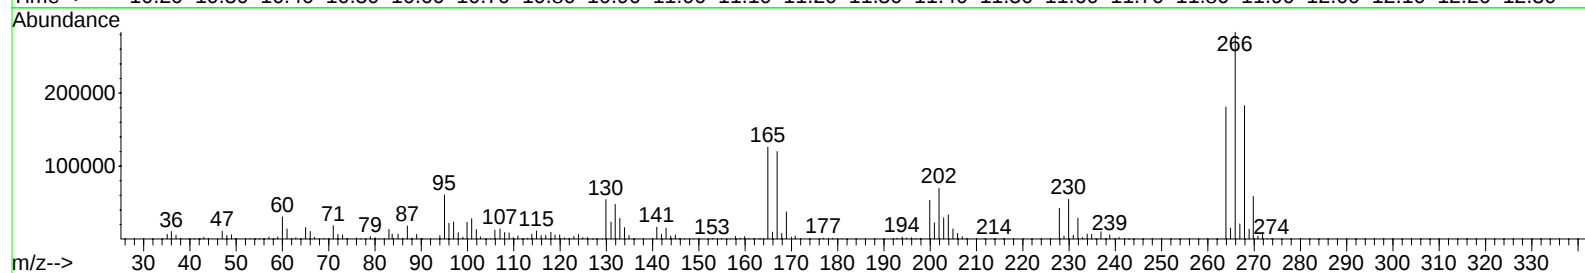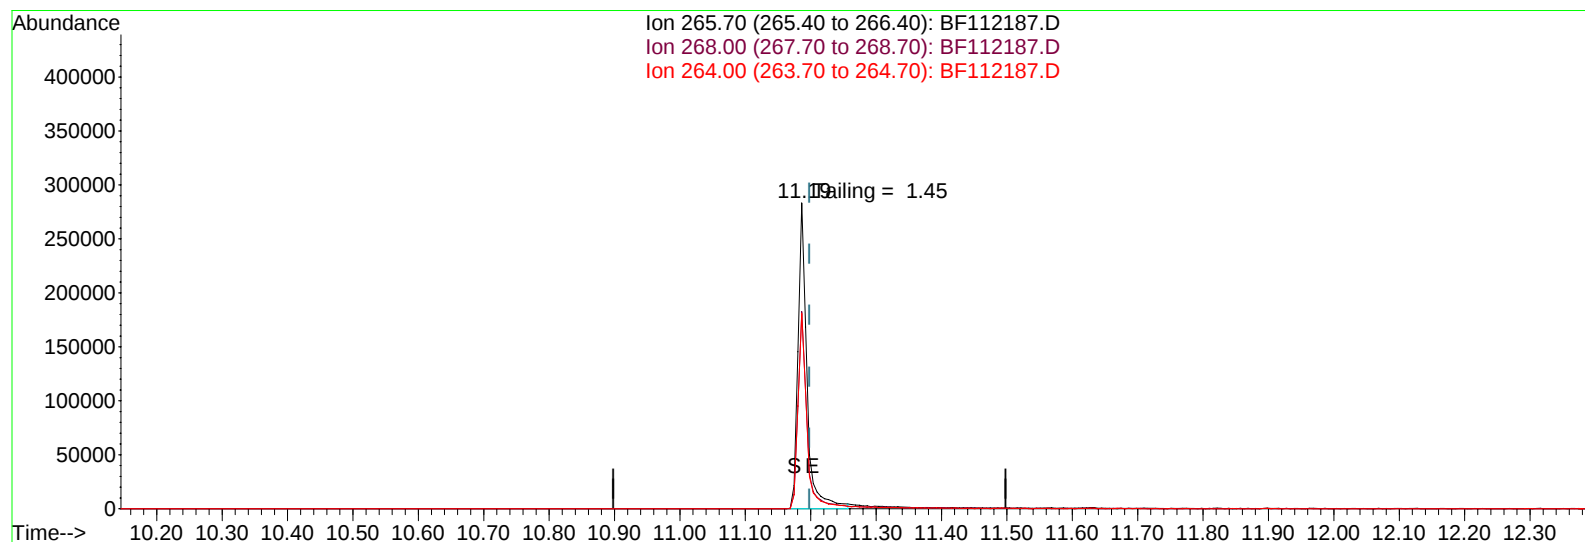

(70) Pentachlorophenol (C)

11.186min (-0.012) 151070.34ng

response 284342

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	64.48
264.00	63.60	63.83
0.00	0.00	0.00