


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012219\
 Data File : BF112187.D
 Acq On : 22 Jan 2019 12:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 19 01:02:12 2019

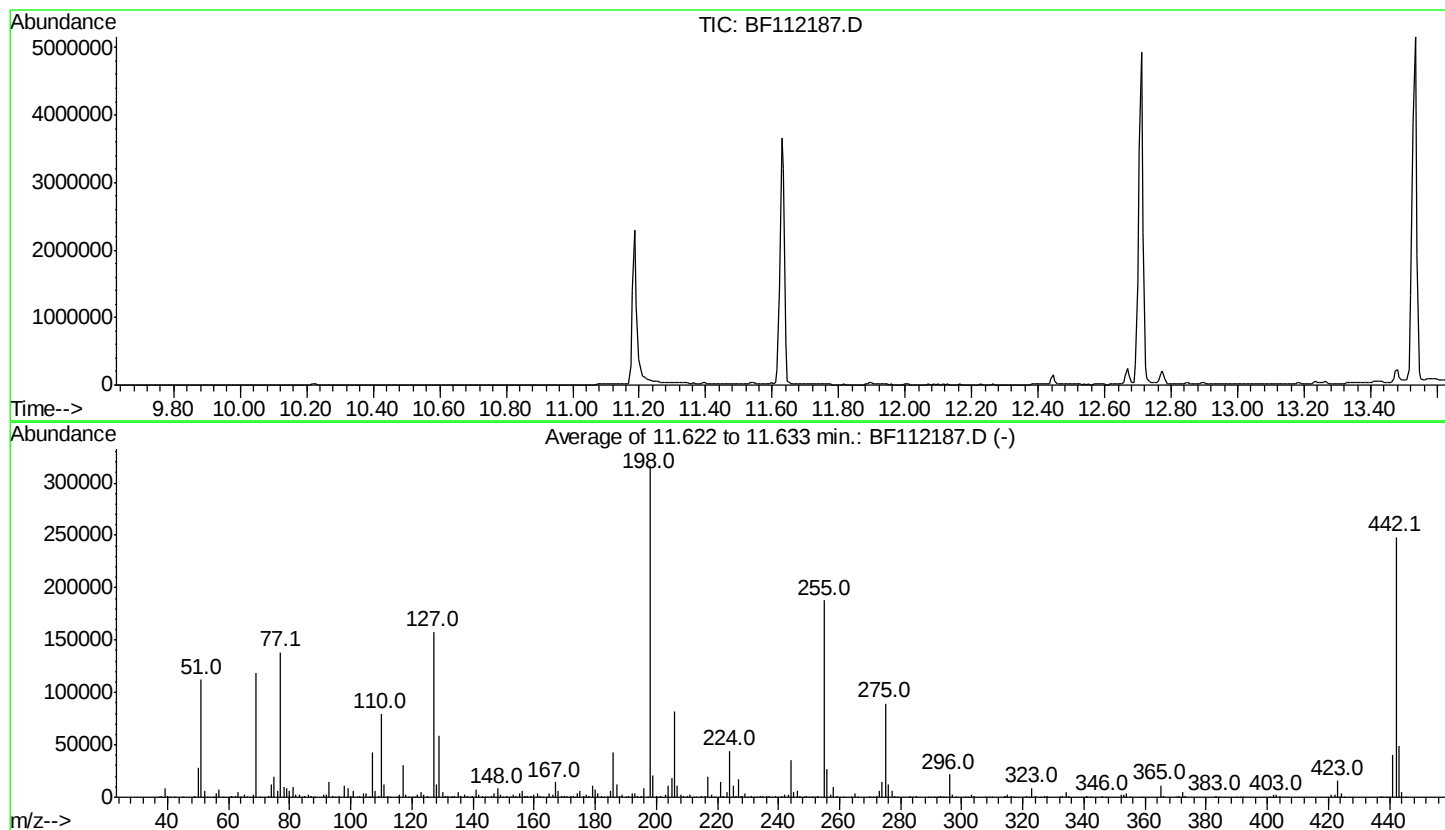

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	112205	PASS
68	69	0.00	2	1.9	2267	PASS
69	198	0.00	100	37.3	118197	PASS
70	69	0.00	2	0.4	447	PASS
127	198	10	80	49.9	157997	PASS
197	198	0.00	2	0.2	550	PASS
198	198	100	100	100.0	316565	PASS
199	198	5	9	6.6	20945	PASS
275	198	10	60	28.3	89597	PASS
365	198	1	100	3.6	11553	PASS
441	198	0.01	100	12.6	39779	PASS
442	198	50	100	78.4	248112	PASS
443	442	15	24	19.9	49314	PASS