


2-Nitrophenol

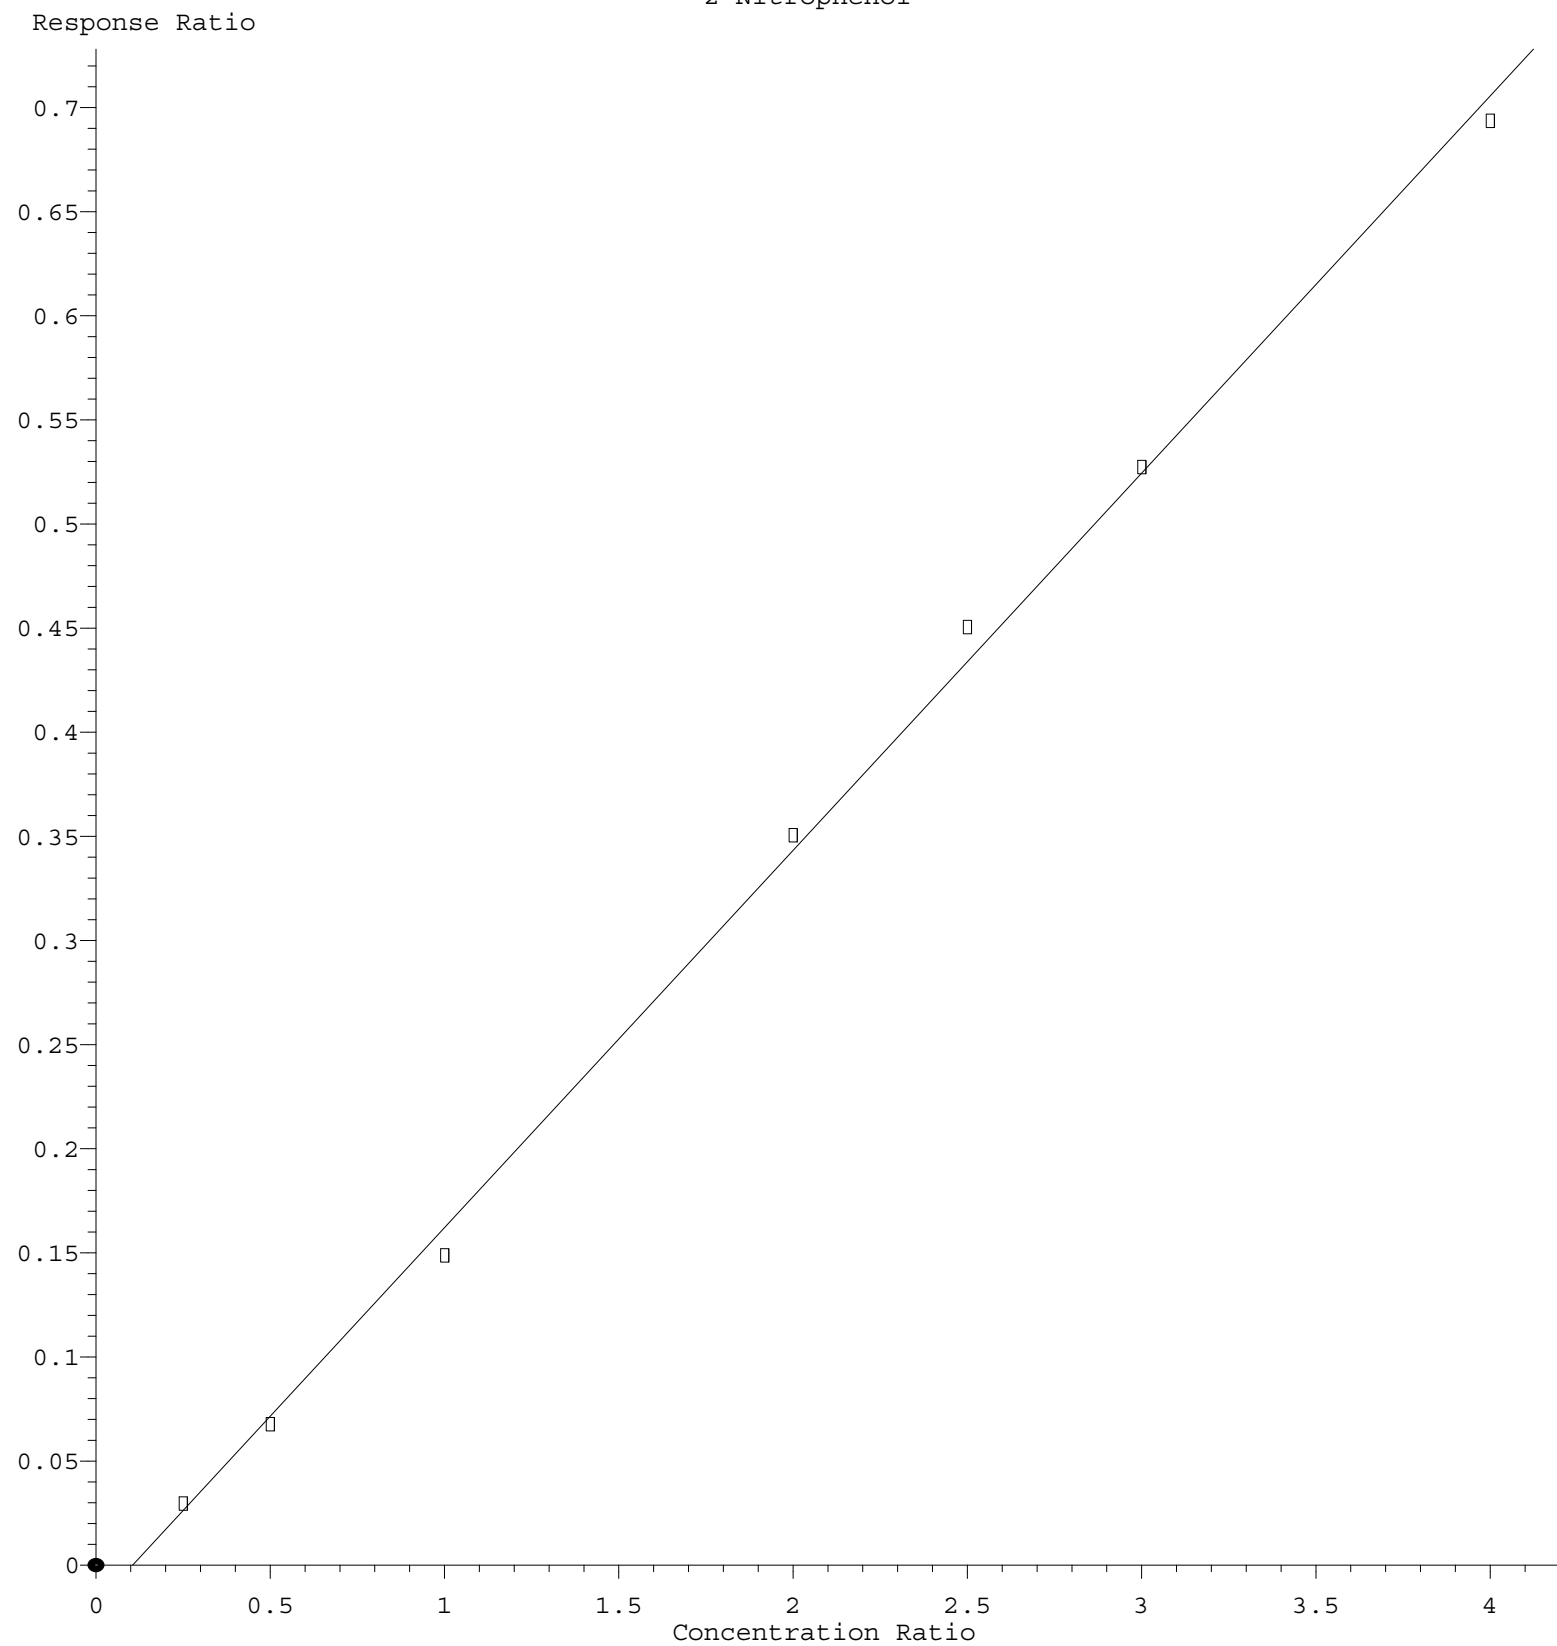

$$\text{Response} = 1.812\text{e-}001 * \text{Amt} - 1.901\text{e-}002$$


Coef of Det (r^2) = 0.998188 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012221.M

Calibration Table Last Updated: Fri Jan 22 15:39:01 2021

Benzoic acid

Response Ratio

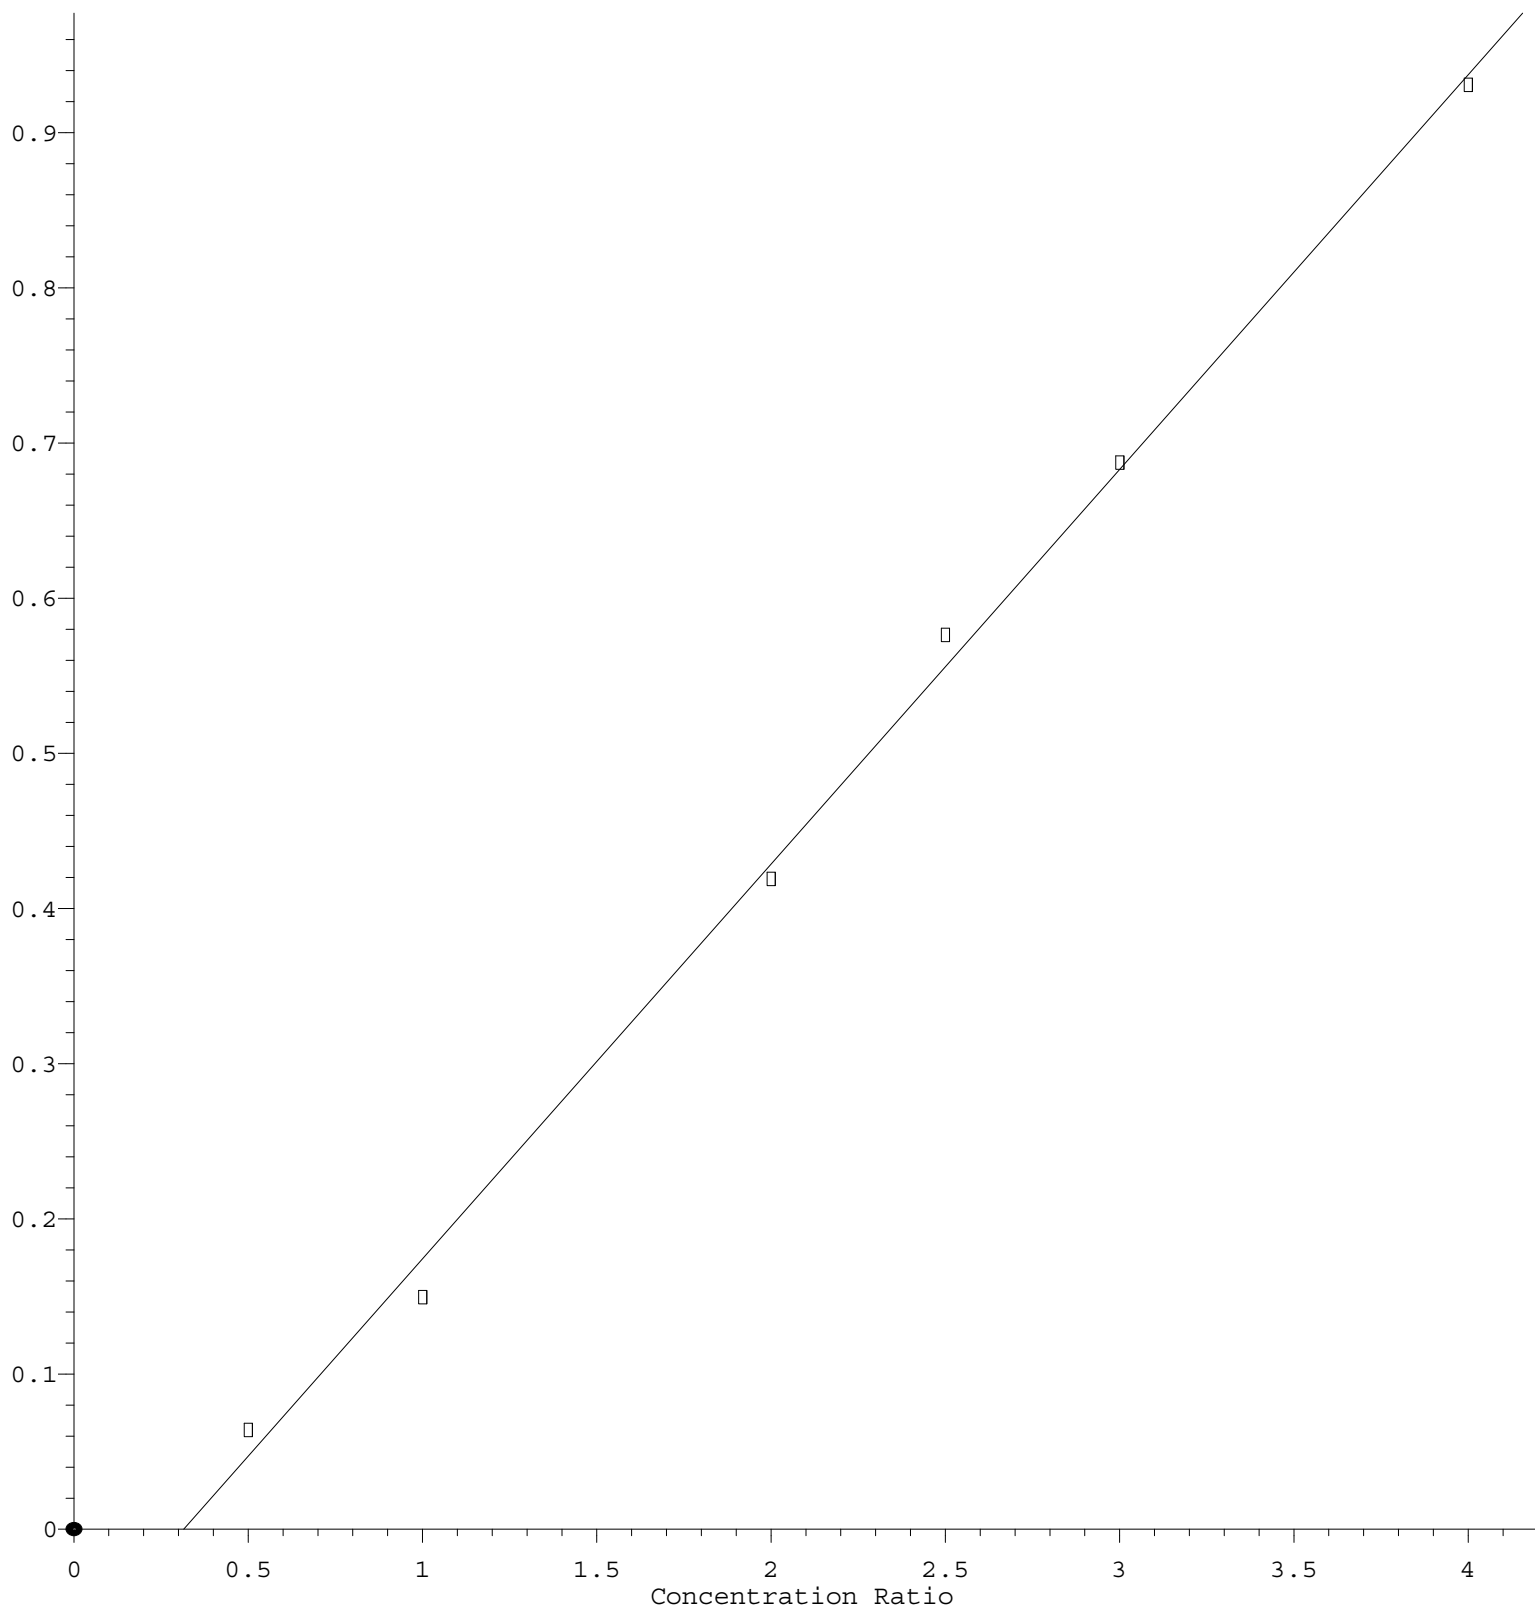


$$\text{Response} = 2.545\text{e-}001 * \text{Amt} - 8.021\text{e-}002$$

Coef of Det (r^2) = 0.997281 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012221.M

Calibration Table Last Updated: Fri Jan 22 15:39:01 2021


2,4-Dinitrophenol

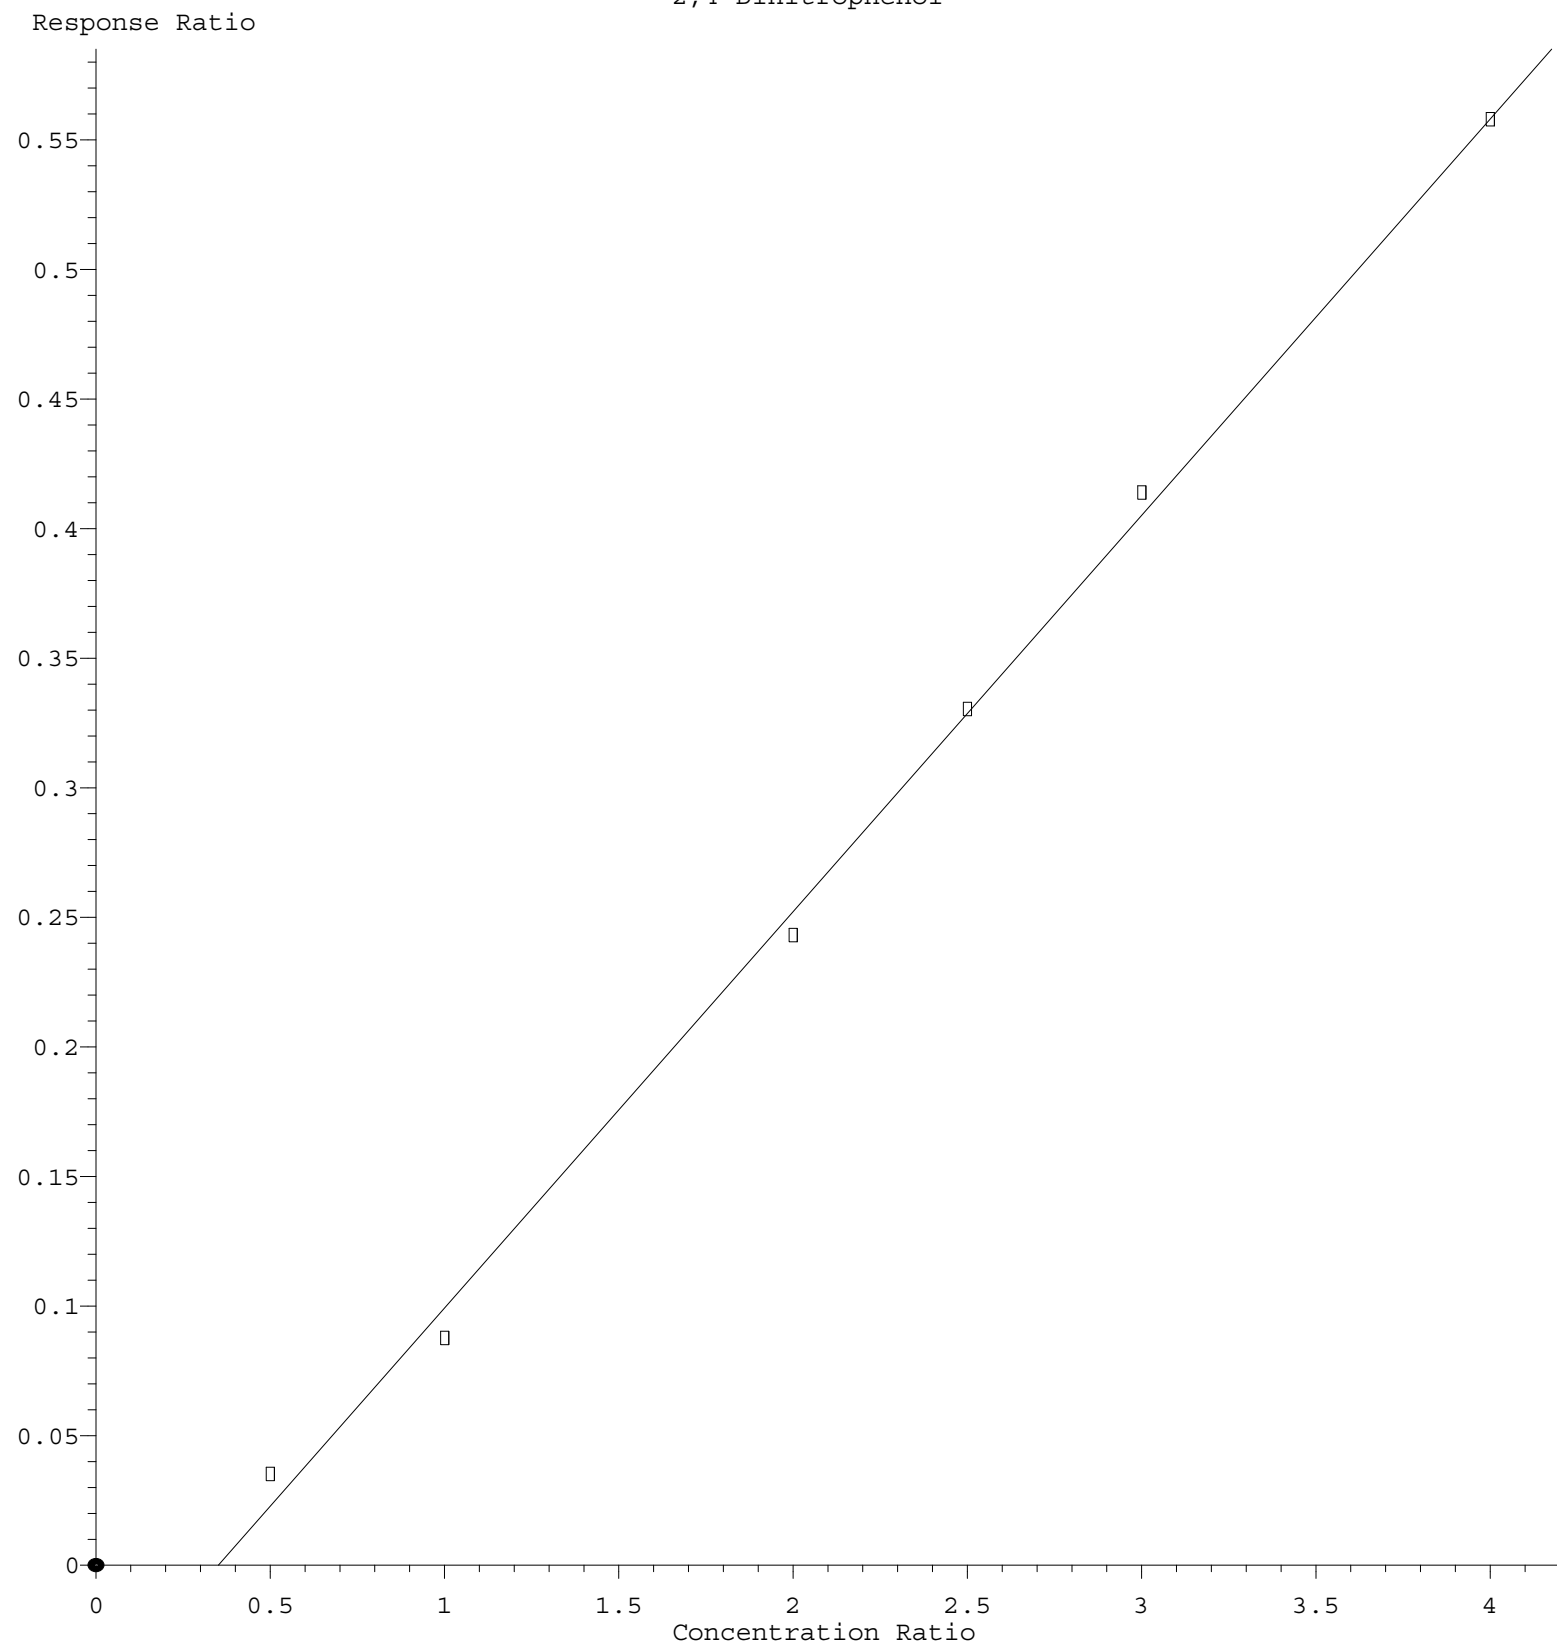

Response = 1.532e-001 * Amt - 5.383e-002
Coef of Det (r^2) = 0.997711 Curve Fit: Linear
Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012221.M
Calibration Table Last Updated: Fri Jan 22 15:39:01 2021

Fluorene

Response Ratio

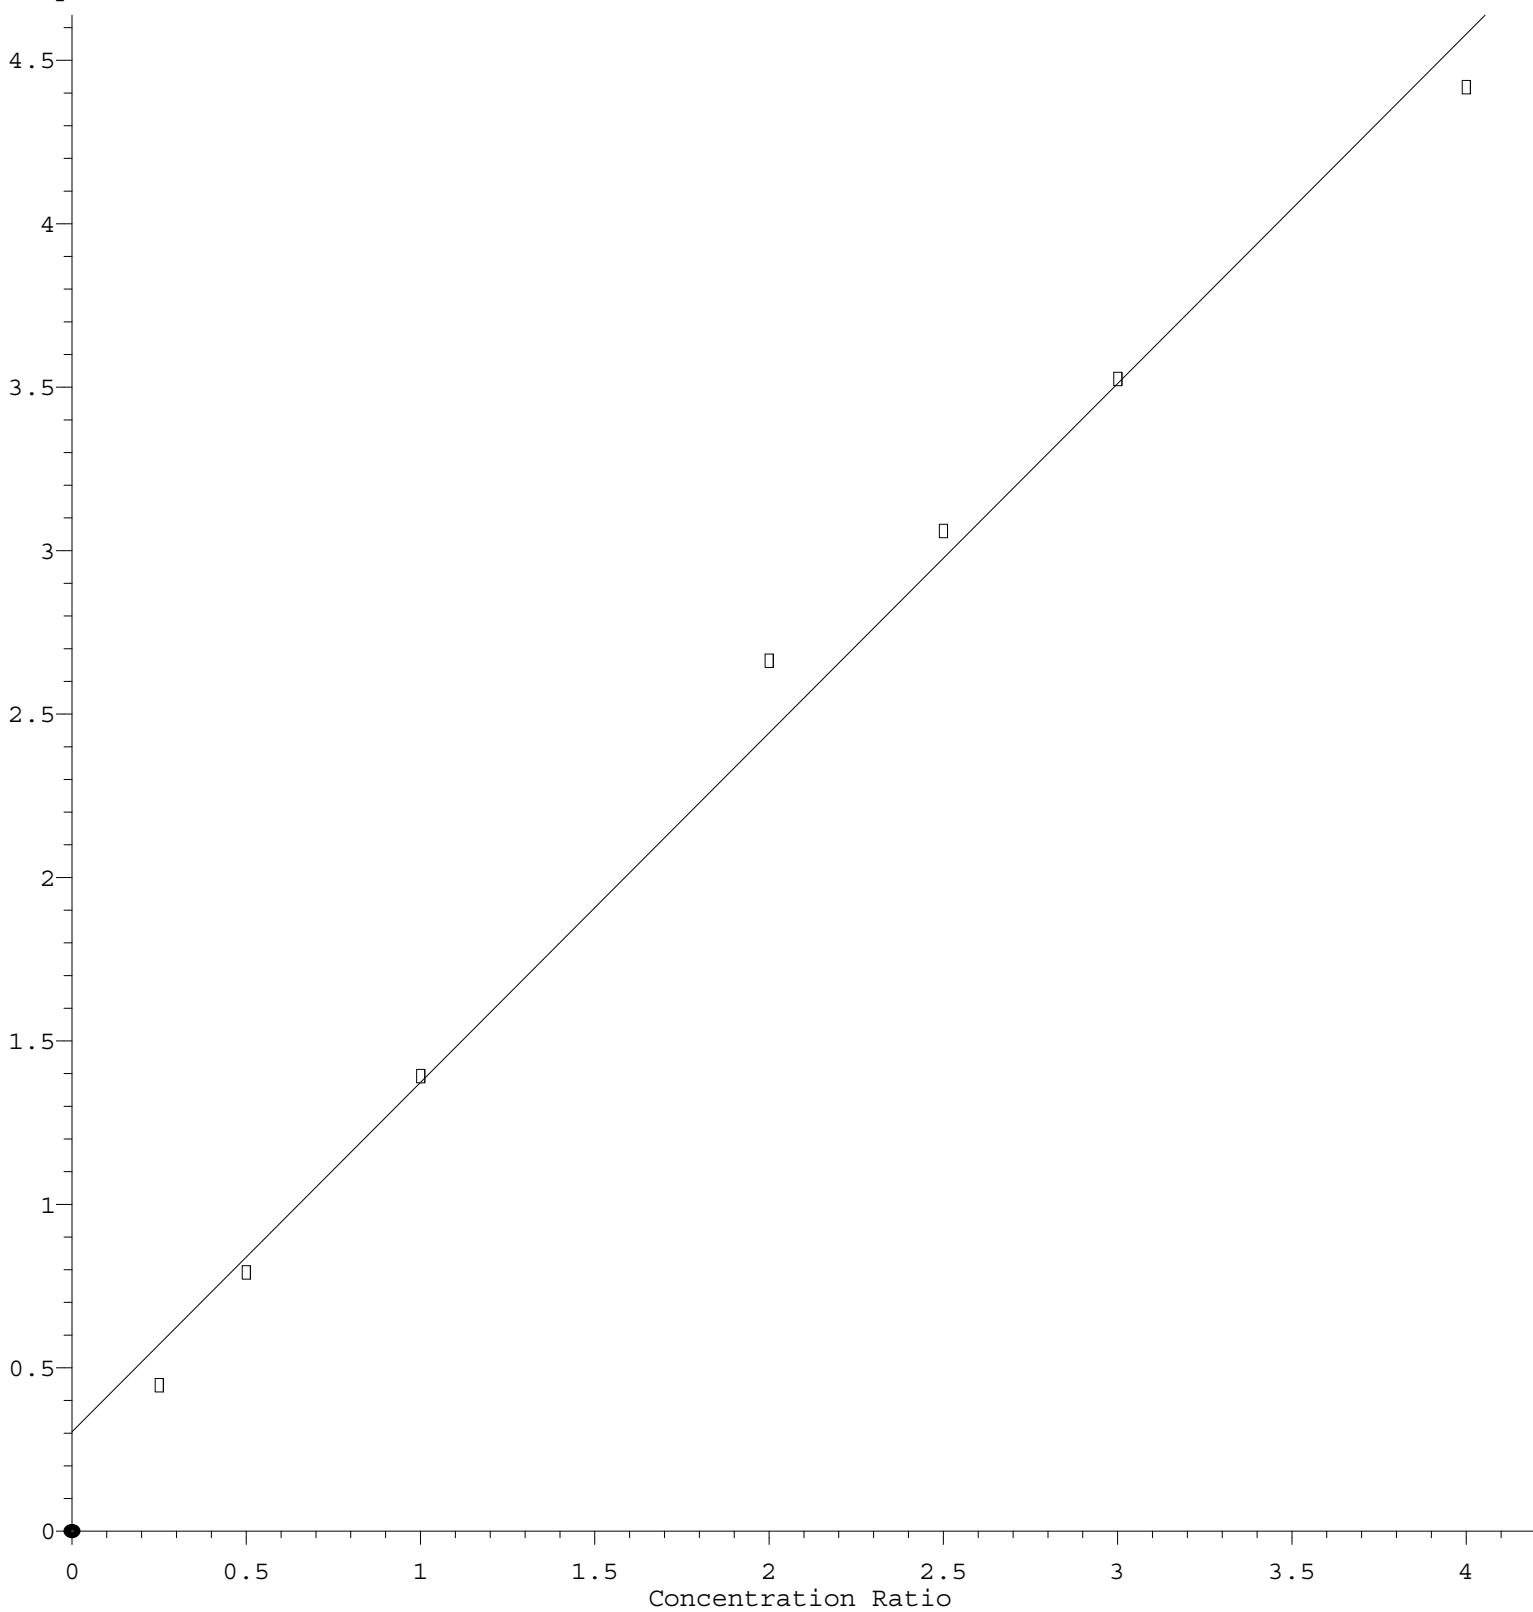


$$\text{Response} = 1.069\text{e}+000 * \text{Amt} + 3.043\text{e}-001$$

Coef of Det (r^2) = 0.992408 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012221.M

Calibration Table Last Updated: Fri Jan 22 15:39:01 2021

4,6-Dinitro-2-methylphenol

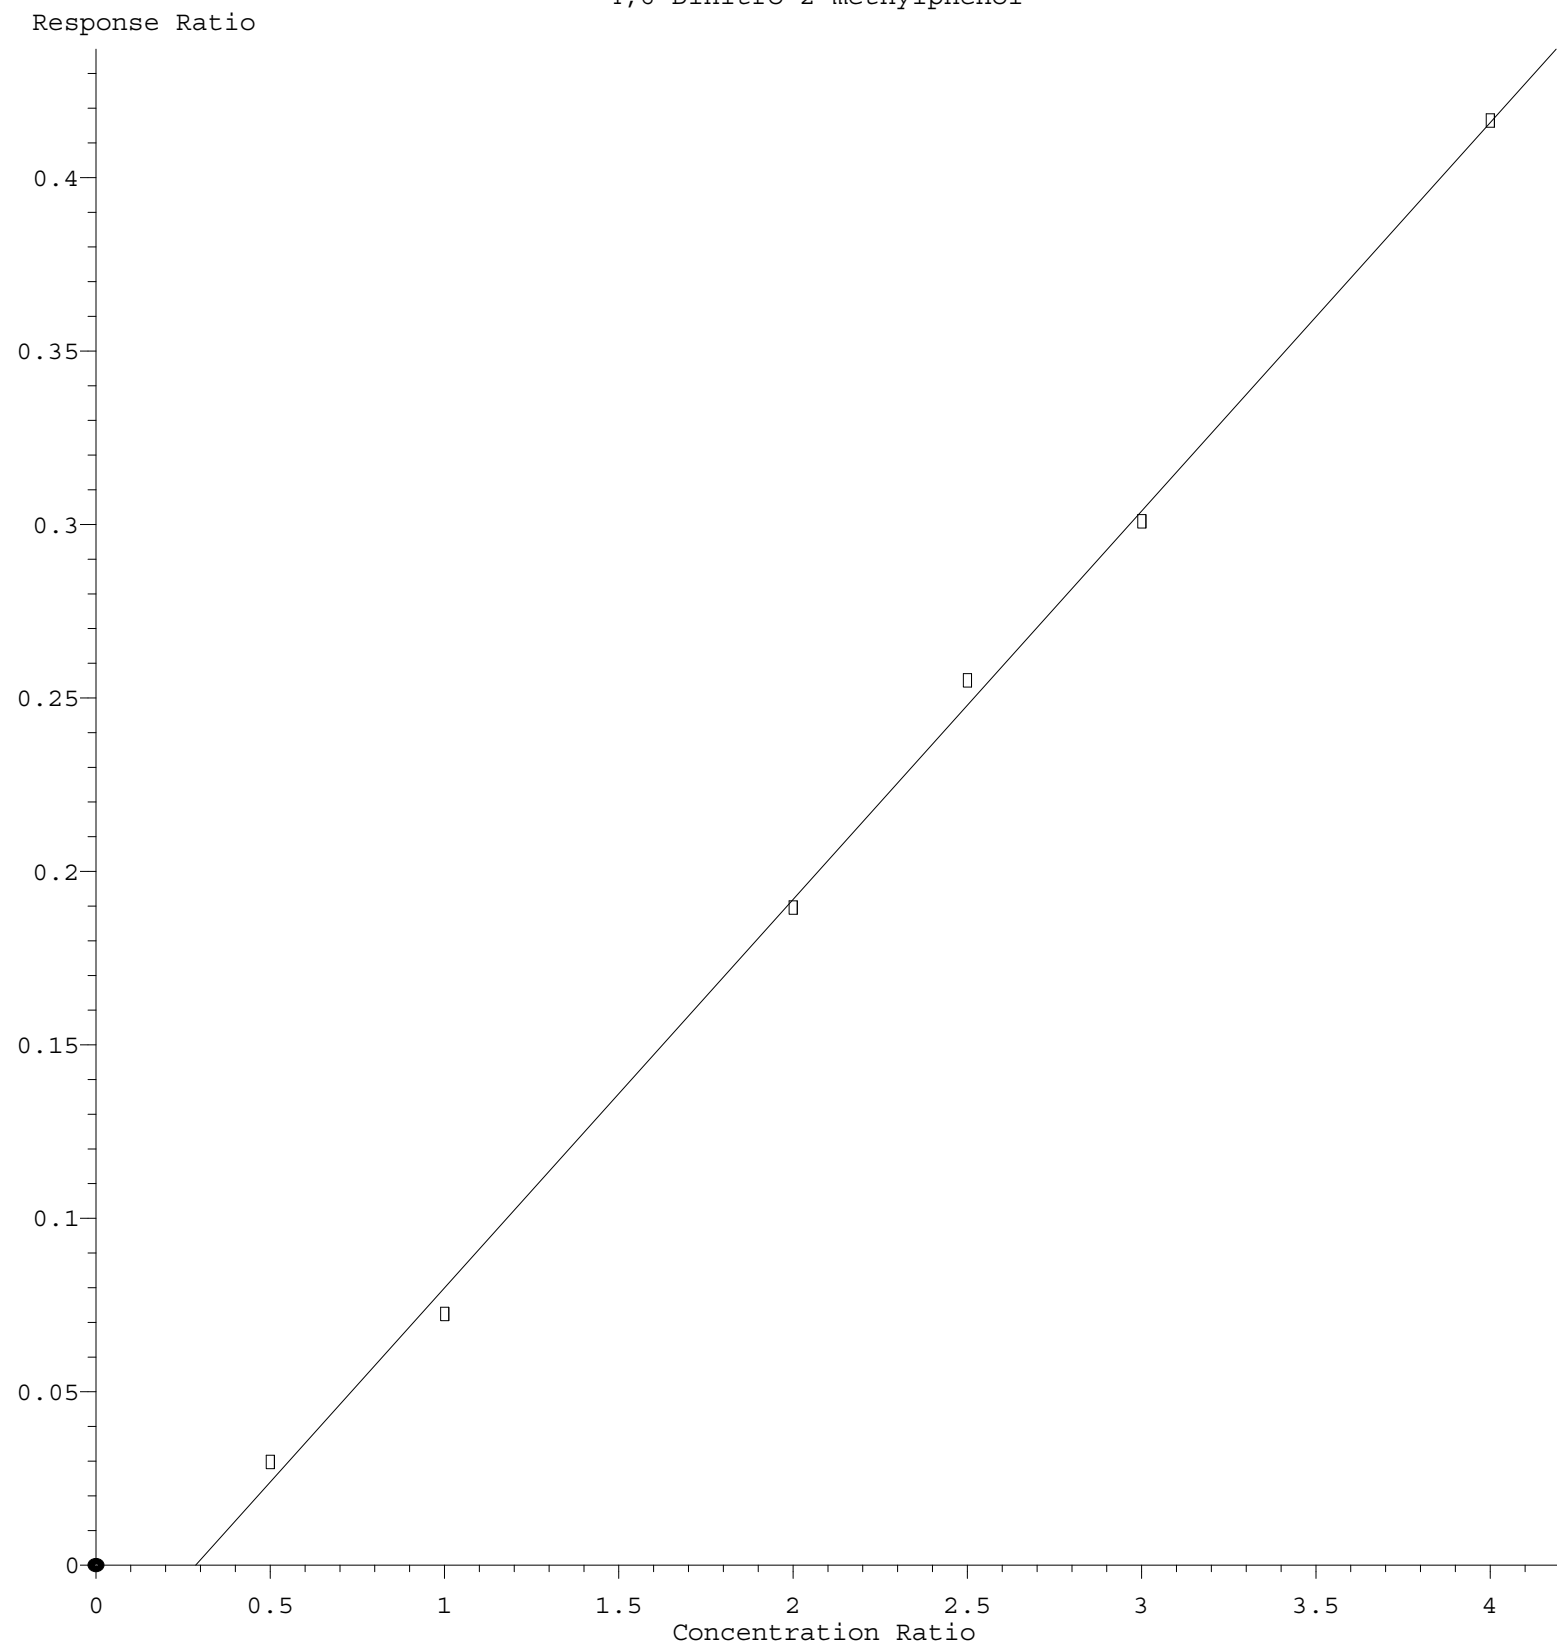

Response = 1.120e-001 * Amt - 3.207e-002
Coef of Det (r^2) = 0.998510 Curve Fit: Linear
Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012221.M
Calibration Table Last Updated: Fri Jan 22 15:39:01 2021