
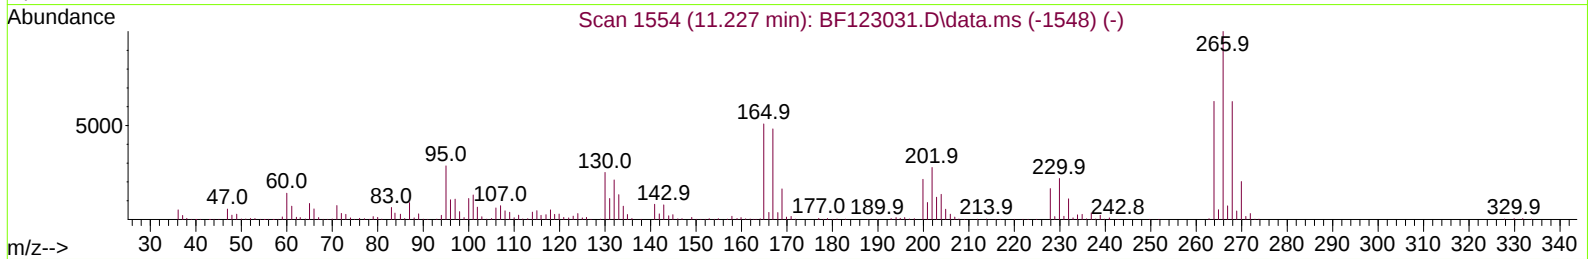
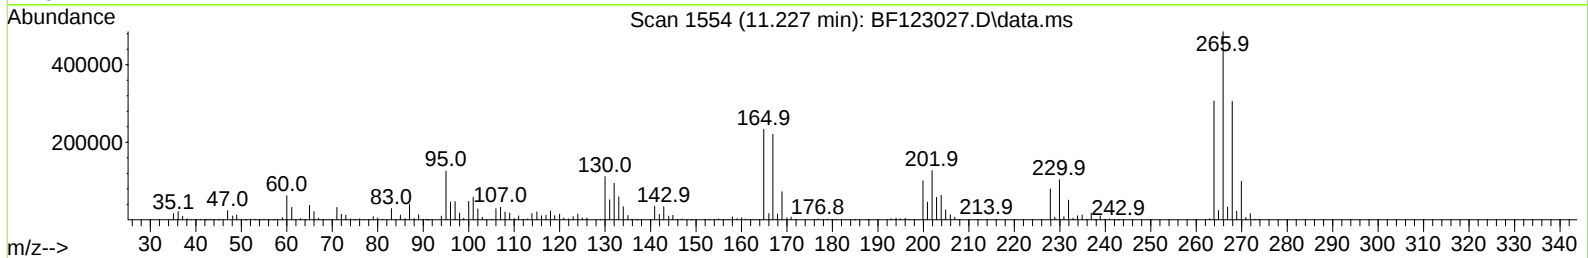


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012221\
 Data File : BF123027.D
 Acq On : 22 Jan 2021 9:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 23:46:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 22 15:39:01 2021
 Response via : Initial Calibration

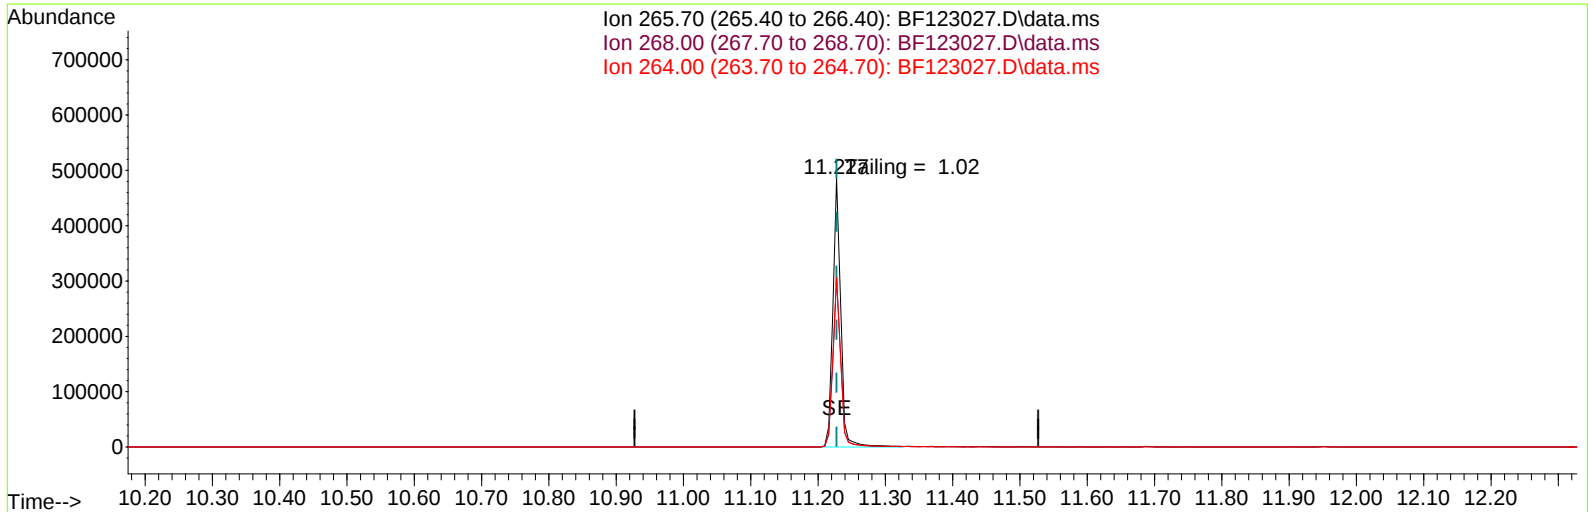




TIC: BF123027.D\data.ms

(70) Pentachlorophenol (C)**11.227min (+ 0.000) 324452.35 ng****response 395960**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.02
264.00	62.30	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012221\
 Data File : BF123027.D
 Acq On : 22 Jan 2021 9:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 23:46:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 22 15:39:01 2021
 Response via : Initial Calibration

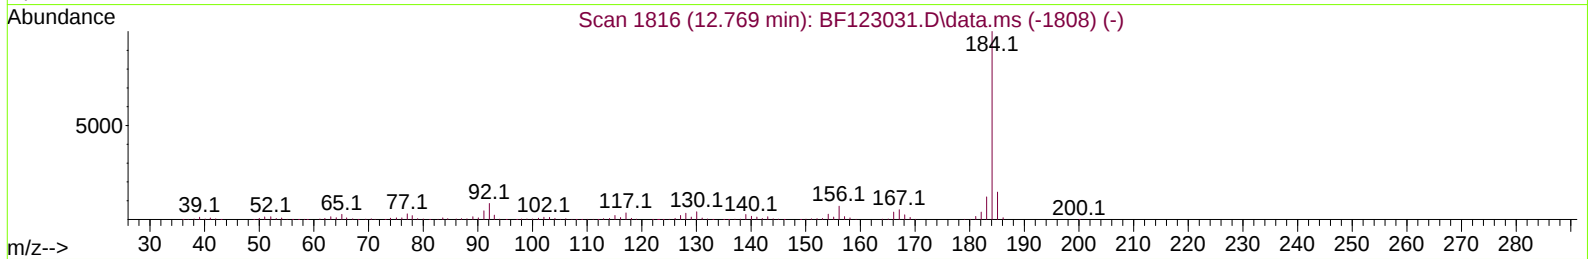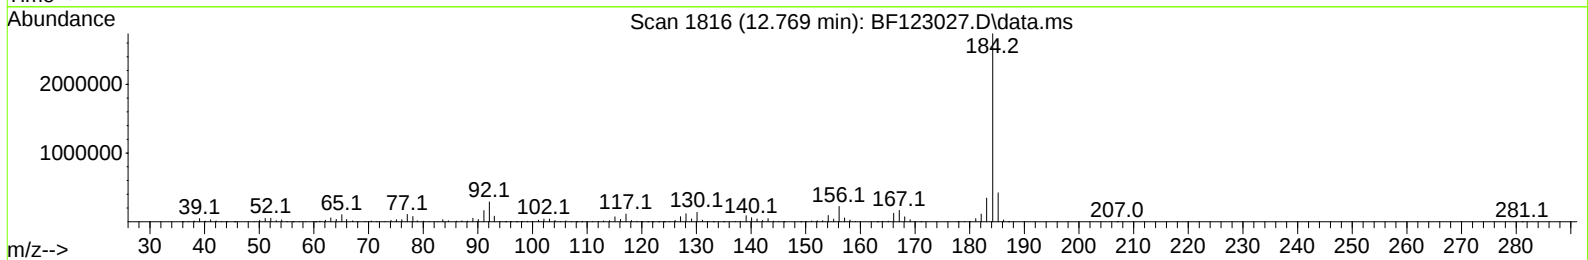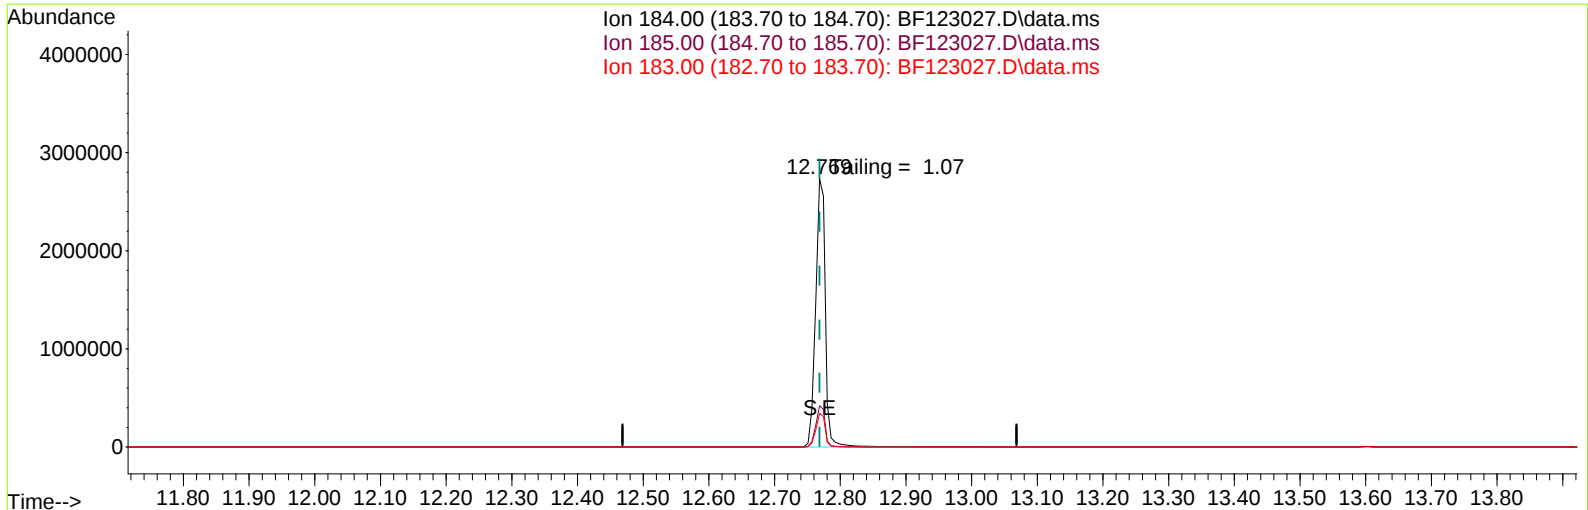

TIC: BF123027.D\data.ms

(77) Benzidine

12.769min (+ 0.000) 31266.38 ng

response 2813617

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.39
183.00	12.10	12.62
0.00	0.00	0.00