
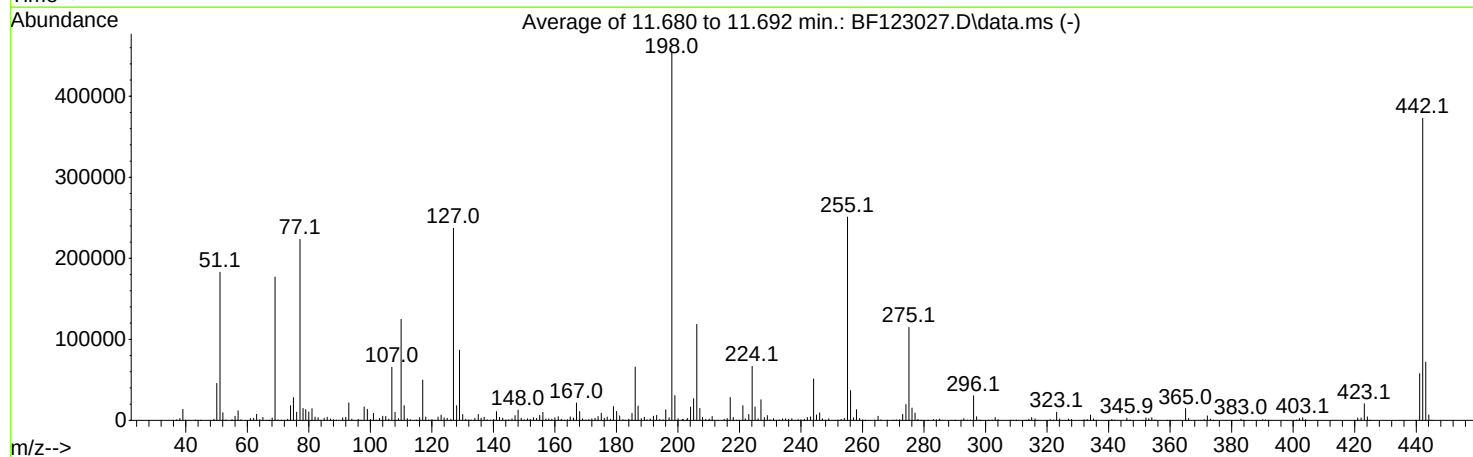


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012221\
 Data File : BF123027.D
 Acq On : 22 Jan 2021 9:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 22 15:39:01 2021

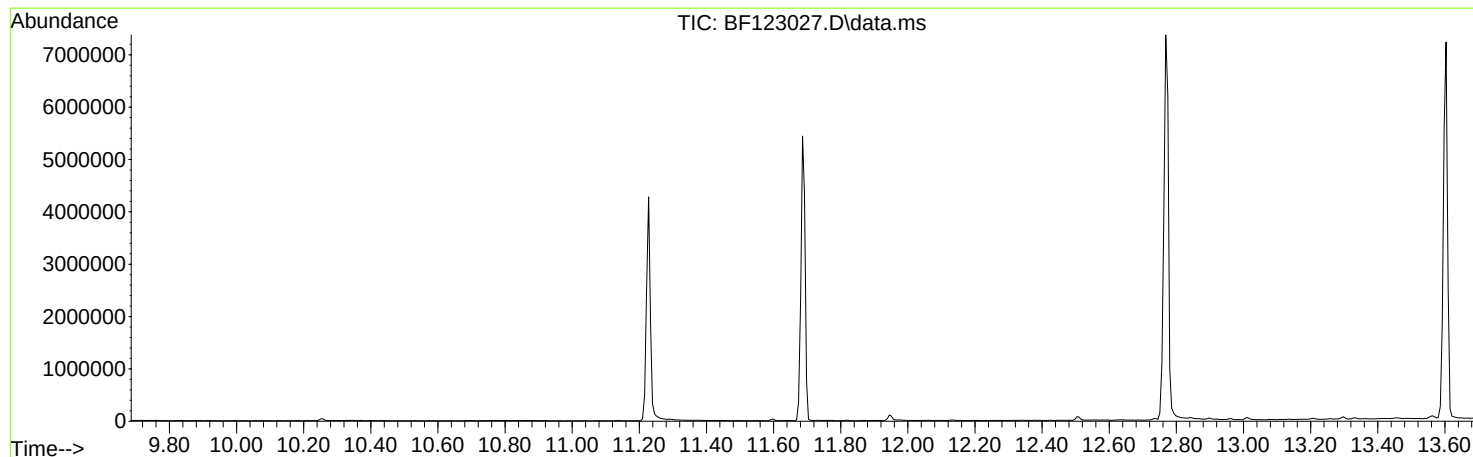

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	182933	PASS
68	69	0.00	2	1.7	3061	PASS
69	198	0.00	100	39.0	176902	PASS
70	69	0.00	2	0.4	698	PASS
127	198	10	80	52.2	237184	PASS
197	198	0.00	2	0.7	3260	PASS
198	198	100	100	100.0	454016	PASS
199	198	5	9	6.7	30555	PASS
275	198	10	60	25.3	114747	PASS
365	198	1	100	3.2	14602	PASS
441	198	0.01	100	12.7	57687	PASS
442	442	50	100	100.0	372880	PASS
443	442	15	24	19.3	71896	PASS