

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012225\
 Data File : BF141237.D
 Acq On : 22 Jan 2025 14:50
 Operator : RC/JU
 Sample : PB166167BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166167BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	560	567	572	rBV	3399590	4758001	70.15%	12.718%
2	6.434	731	738	743	rBV	3276101	4755727	70.11%	12.712%
3	6.804	796	801	806	rBV	793733	969391	14.29%	2.591%
4	7.363	889	896	902	rBV	2221583	3215334	47.40%	8.594%
5	8.086	1013	1019	1024	rBV	1007013	1312243	19.35%	3.508%
6	9.163	1195	1202	1207	rBV	4422926	6133566	90.43%	16.395%
7	9.839	1311	1317	1323	rBV	1148607	1528463	22.53%	4.085%
8	10.633	1445	1452	1457	rBV	3073773	4066300	59.95%	10.869%
9	11.327	1565	1570	1576	rBV	1214183	1563345	23.05%	4.179%
10	12.921	1835	1841	1846	rBV	5070184	6782908	100.00%	18.130%
11	13.980	2015	2021	2030	rBV	986204	1311573	19.34%	3.506%
12	15.456	2266	2272	2279	rBV	623686	1015193	14.97%	2.714%




Sum of corrected areas: 37412044

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012225\
Data File : BF141237.D
Acq On : 22 Jan 2025 14:50
Operator : RC/JU
Sample : PB166167BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166167BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

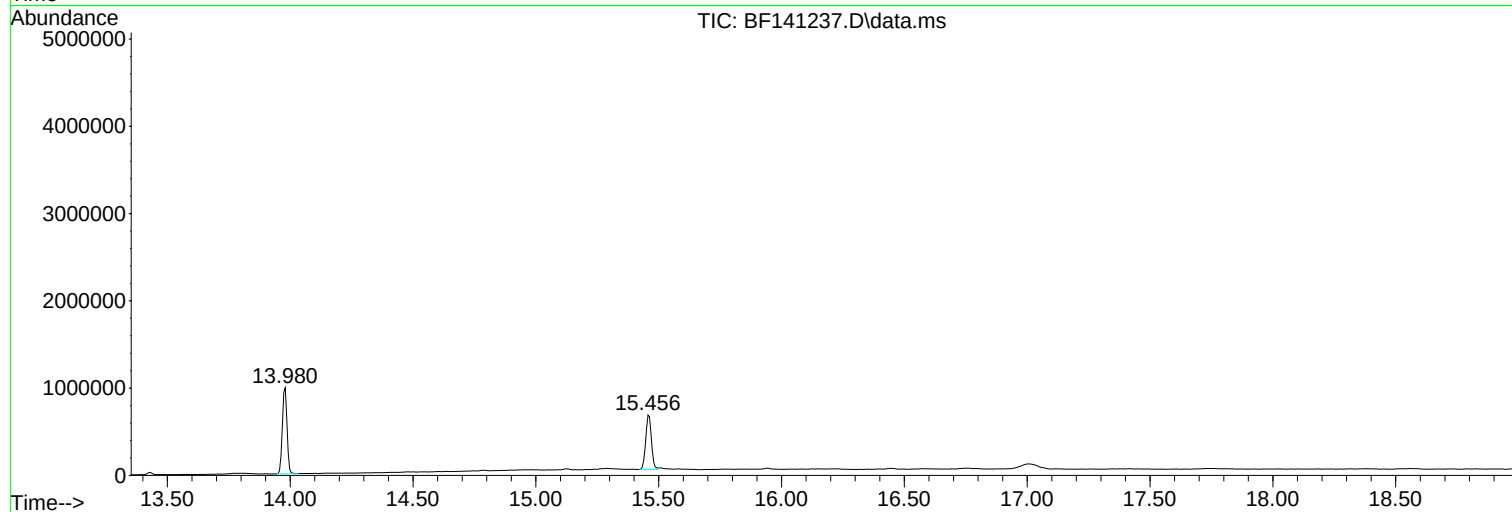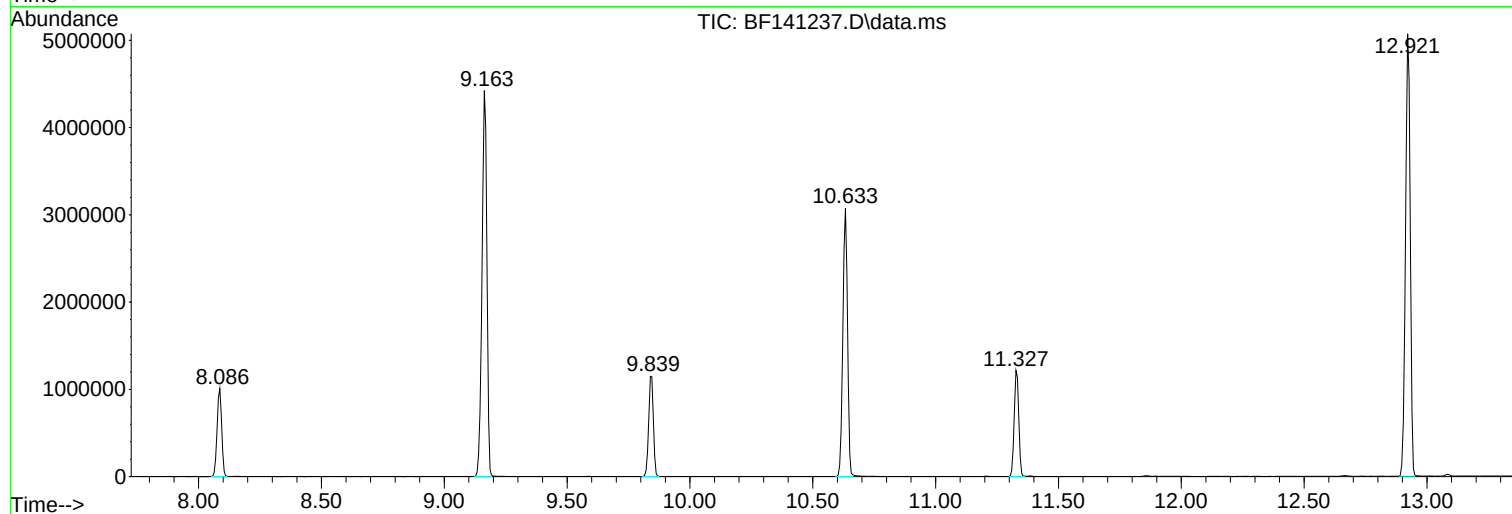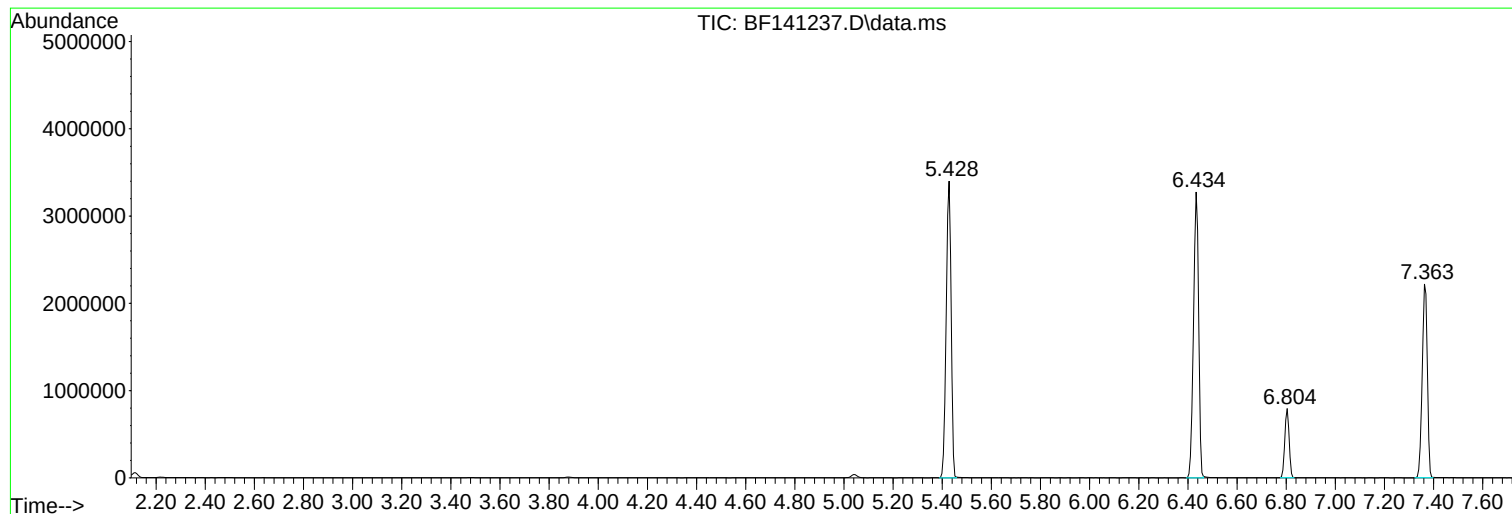

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012225\
Data File : BF141237.D
Acq On : 22 Jan 2025 14:50
Operator : RC/JU
Sample : PB166167BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166167BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012225\
Data File : BF141237.D
Acq On : 22 Jan 2025 14:50
Operator : RC/JU
Sample : PB166167BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166167BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------