


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012225\
Data File : BF141235.D
Acq On : 22 Jan 2025 13:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

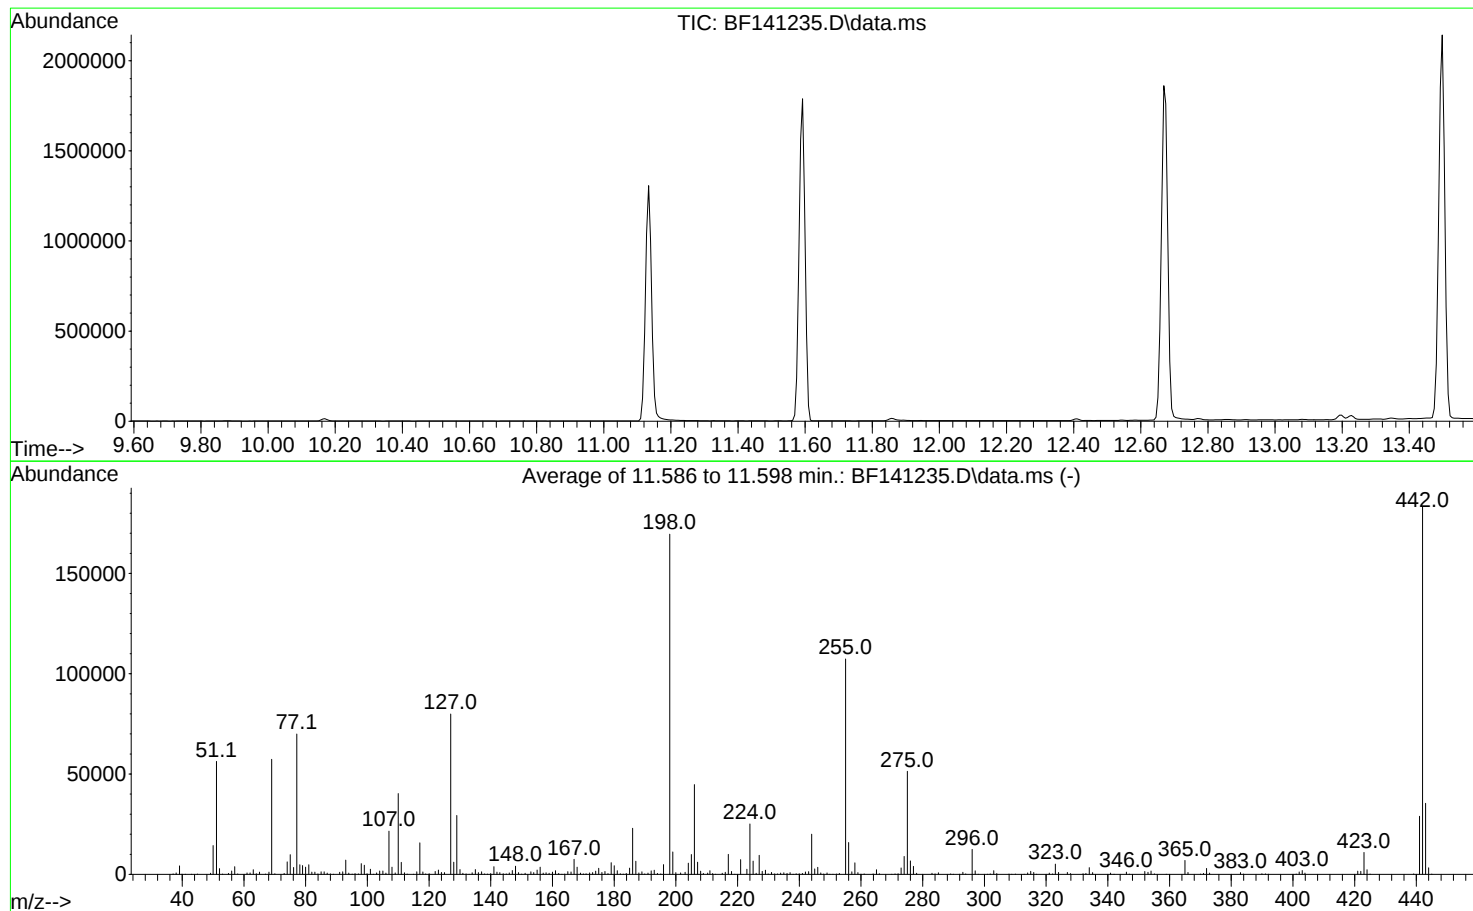

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	56301	PASS
68	69	0.00	2	2.0	1122	PASS
69	198	0.00	100	33.8	57381	PASS
70	69	0.00	2	0.5	296	PASS
127	198	10	80	47.1	79941	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	169579	PASS
199	198	5	9	6.6	11146	PASS
275	198	10	60	30.3	51336	PASS
365	198	1	100	4.1	6929	PASS
441	198	0.01	100	17.1	28936	PASS
442	442	50	100	100.0	183360	PASS
443	442	15	24	19.3	35437	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/22/2025	BNA_F	<u>BF141235.D</u>
Compound Name	Response	Retention Time
DDT	540734	13.498
DDD	12681	13.198
DDE	664	12.864
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13345	554079	2.41

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012225\
Data File : BF141235.D
Acq On : 22 Jan 2025 13:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 22 15:09:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

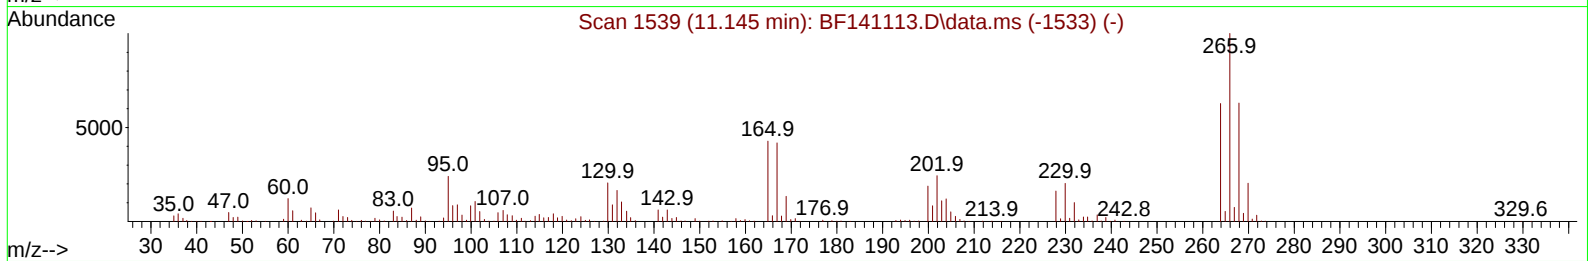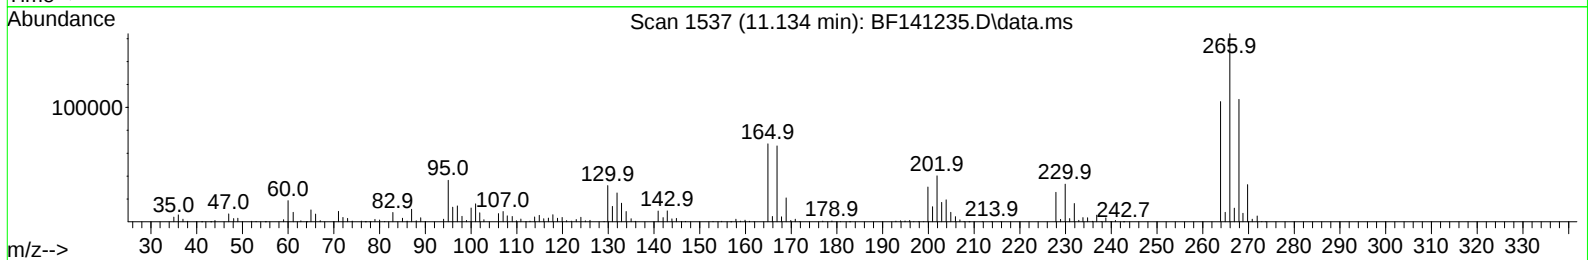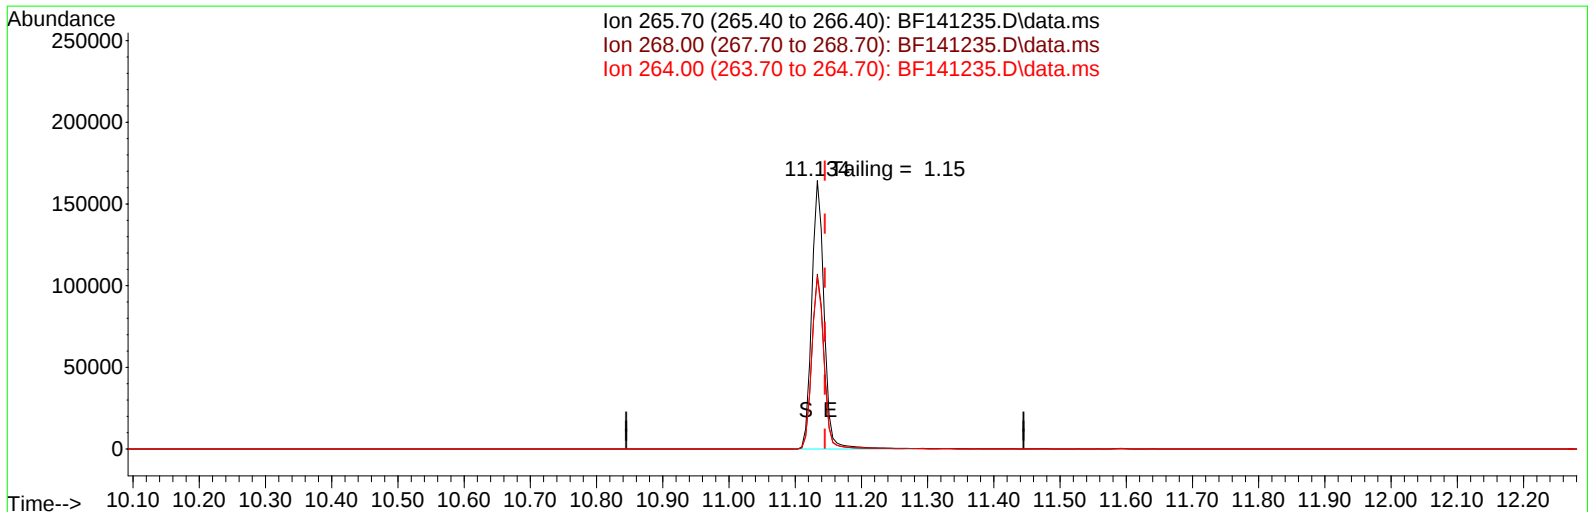

TIC: BF141235.D\data.ms

(70) Pentachlorophenol (C)

11.134min (-0.012) 56694.73 ng




response 213582

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.12
264.00	62.70	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012225\
Data File : BF141235.D
Acq On : 22 Jan 2025 13:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 22 15:09:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

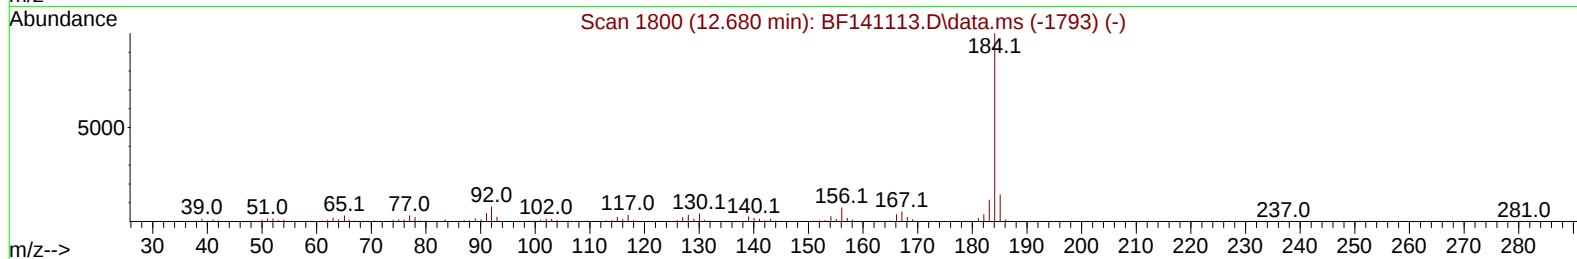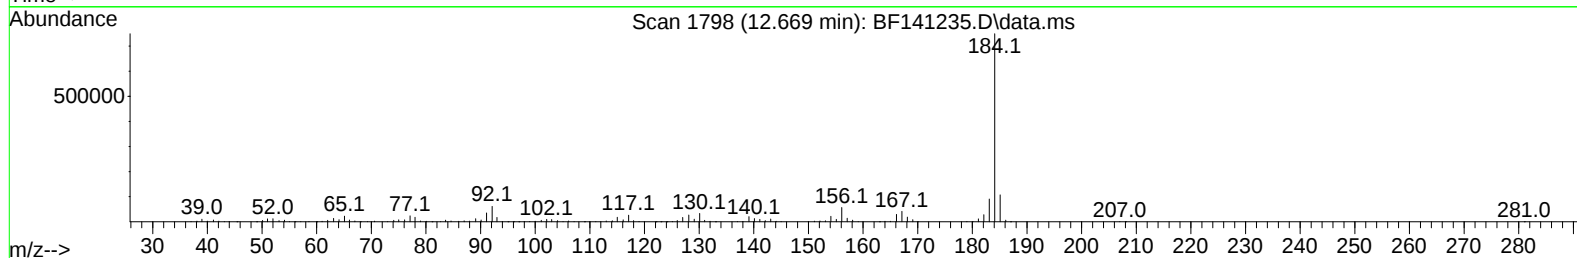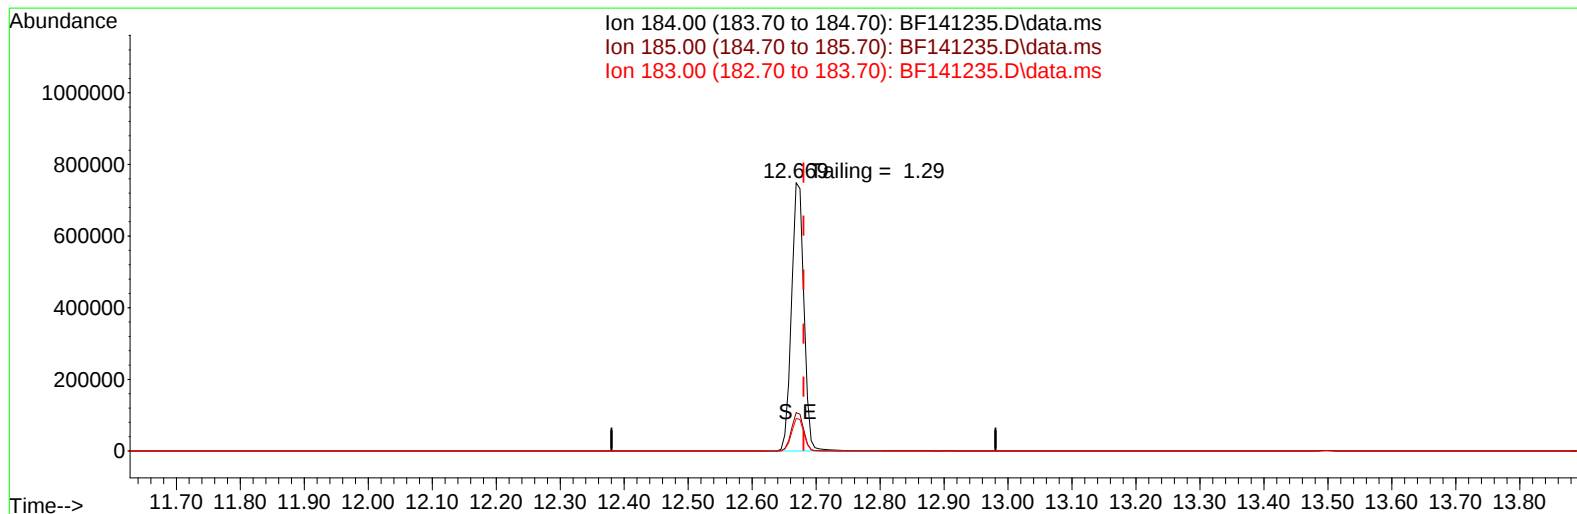

TIC: BF141235.D\data.ms

(77) Benzidine

12.669min (-0.012) 98791.12 ng

response 1011275

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.34
183.00	11.50	12.09
0.00	0.00	0.00