
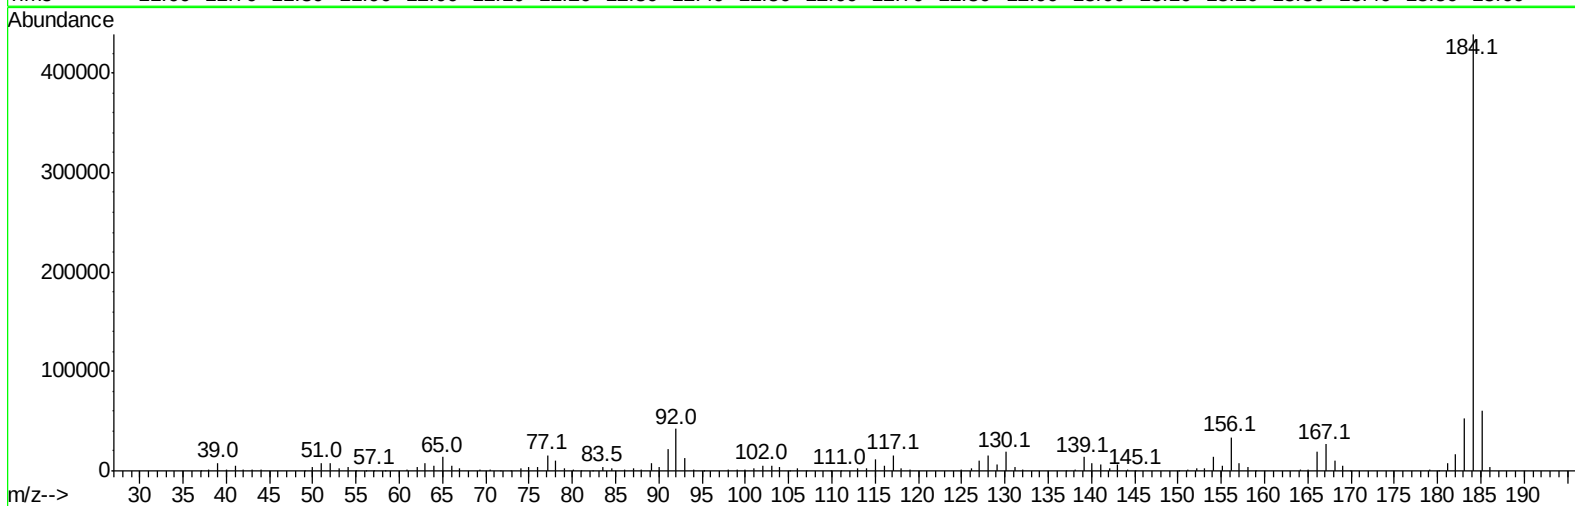


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012318\
Data File : BF102333.D
Acq On : 23 Jan 2018 9:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 07:46:58 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 00:43:41 2018
Response via : Initial Calibration

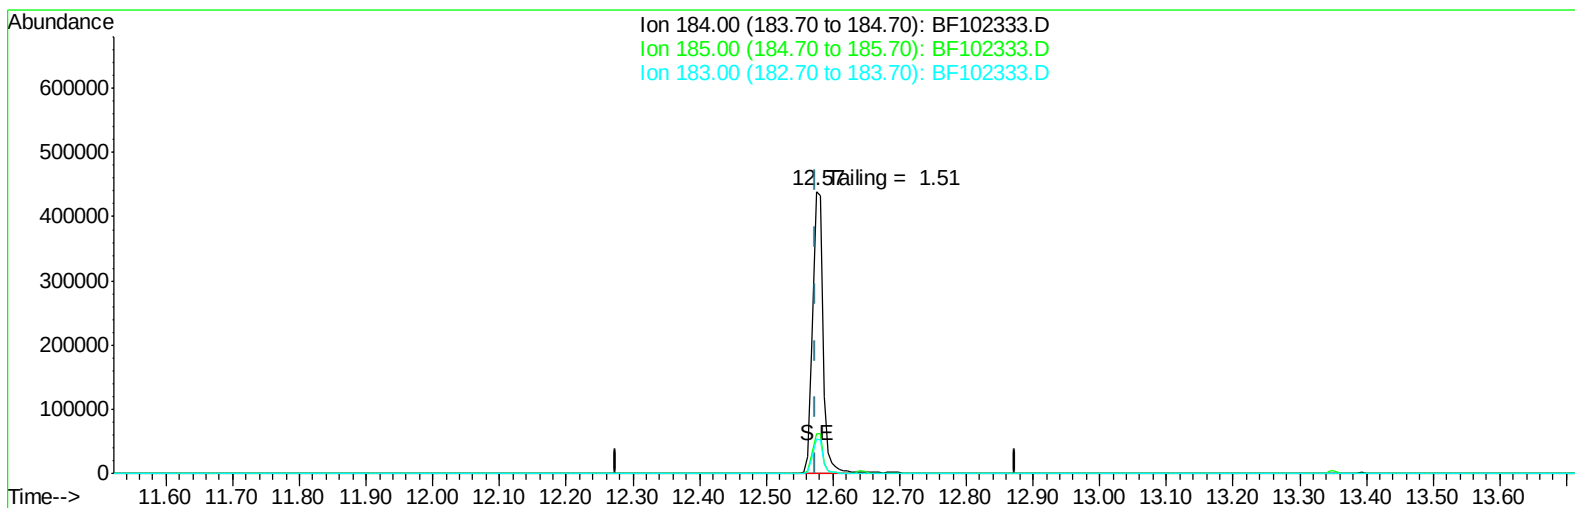

TIC: BF102333.D

(76) Benzidine



12.575min (+0.000) 0.00ng

response 460479

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.93
183.00	11.60	12.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012318\
Data File : BF102333.D
Acq On : 23 Jan 2018 9:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 07:46:58 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 00:43:41 2018
Response via : Initial Calibration

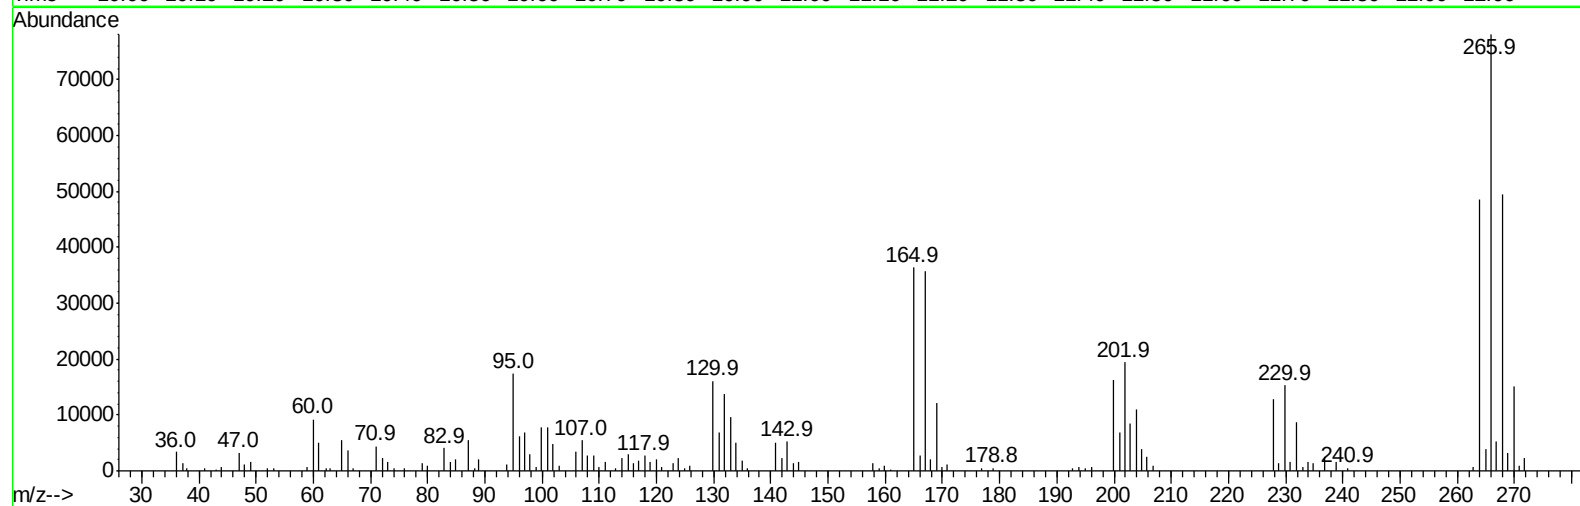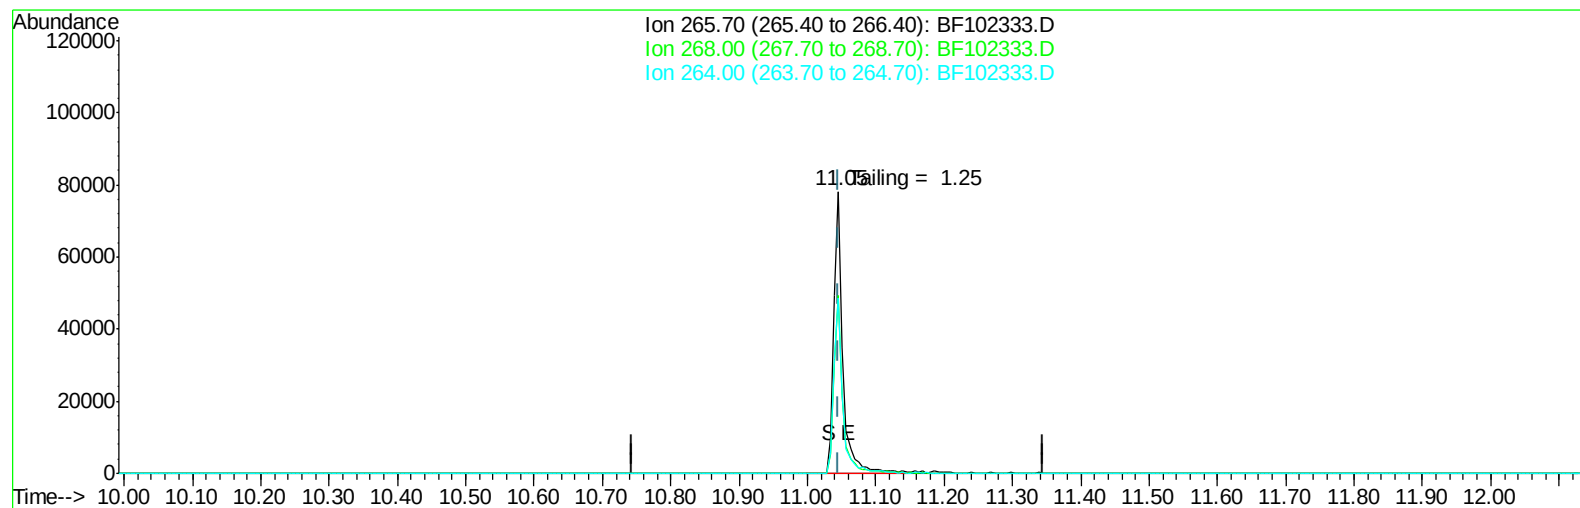

TIC: BF102333.D

(69) Pentachlorophenol (C)

11.045min (+0.000) 35798.38ng

response 73582

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.40
264.00	61.90	62.14
0.00	0.00	0.00