
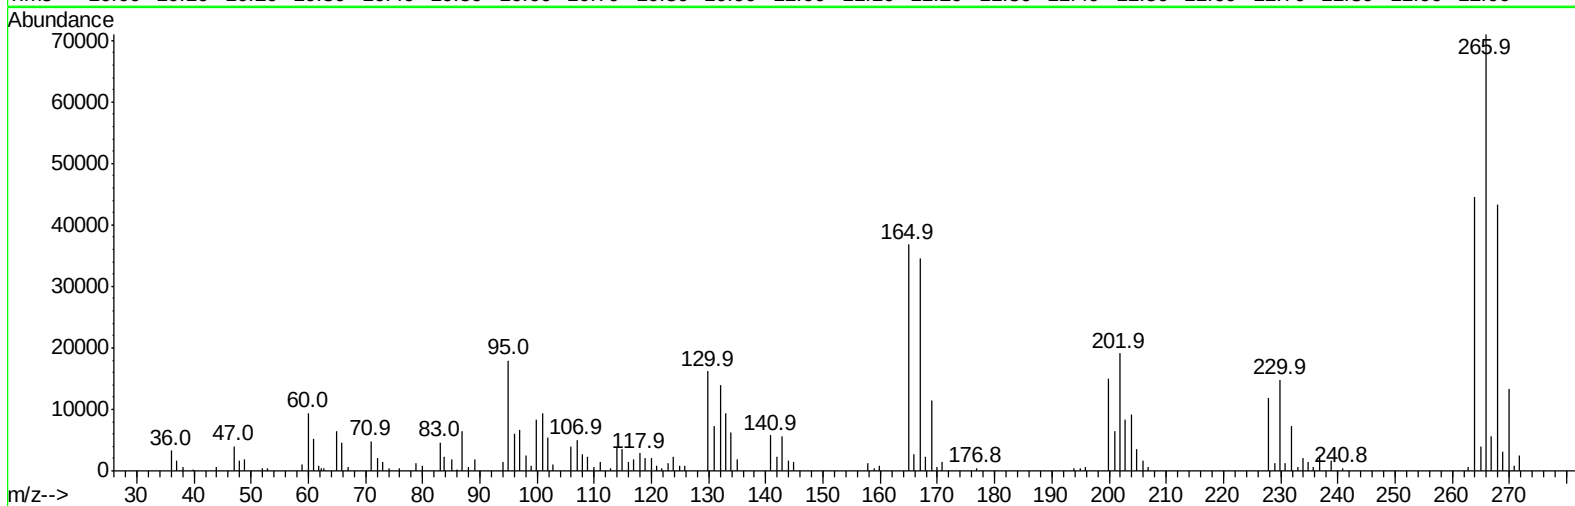


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012318\
Data File : BF102347.D
Acq On : 23 Jan 2018 17:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 07:51:38 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 00:43:41 2018
Response via : Initial Calibration

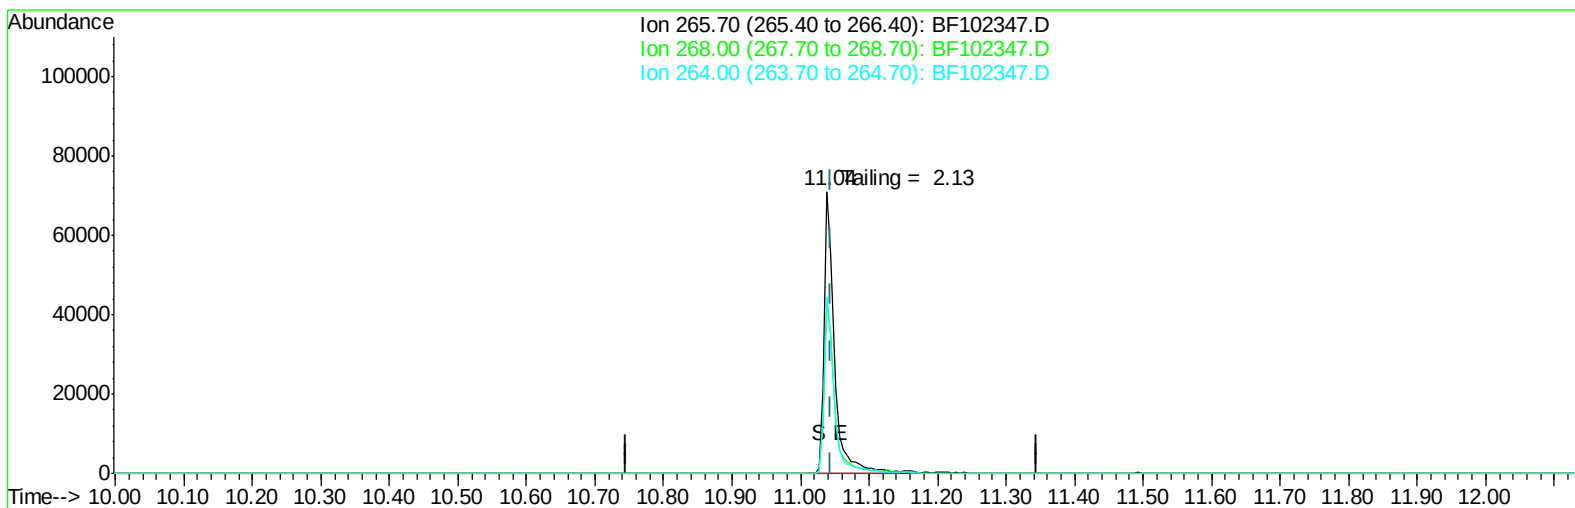

TIC: BF102347.D

(69) Pentachlorophenol (C)



11.039min (-0.006) 29143.06ng

response 72620

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.86
264.00	61.90	62.66
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012318\
Data File : BF102347.D
Acq On : 23 Jan 2018 17:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 07:51:38 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 00:43:41 2018
Response via : Initial Calibration

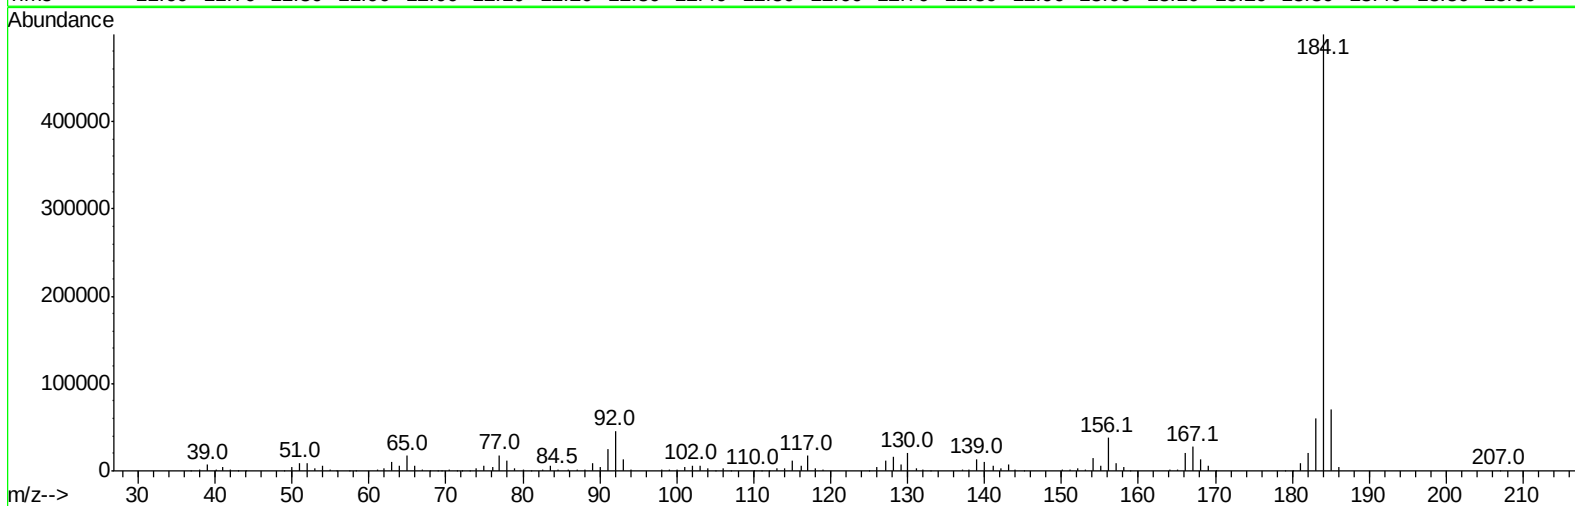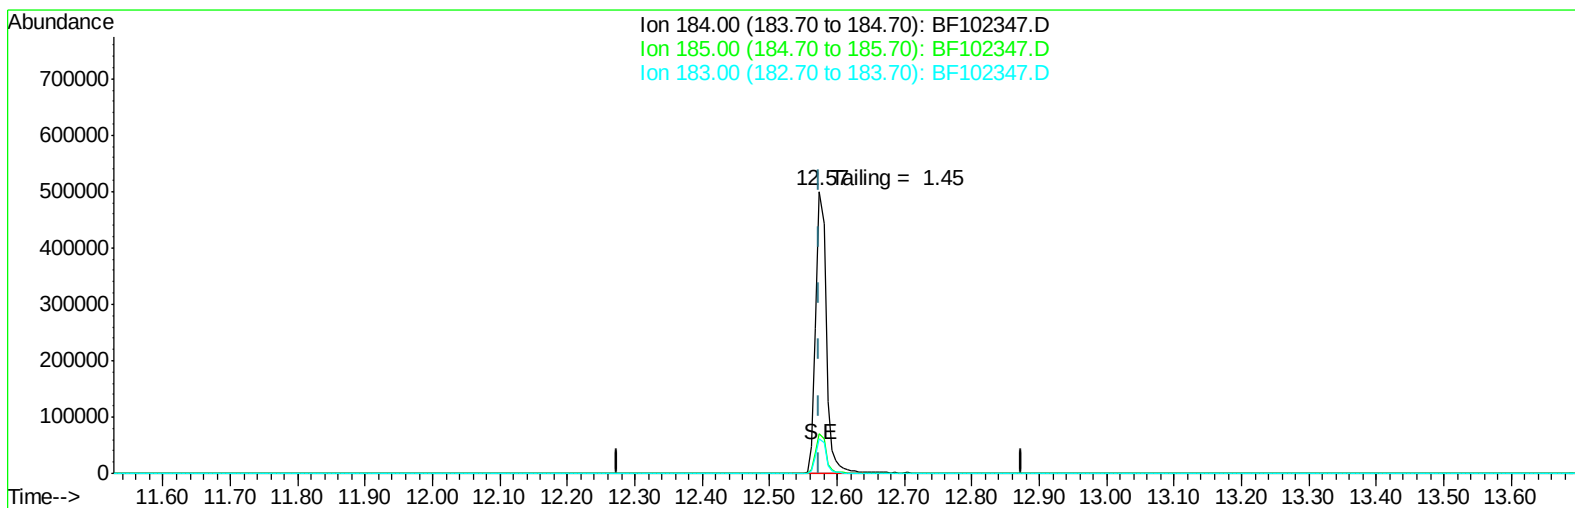

TIC: BF102347.D

(76) Benzidine

12.574min (-0.000) 0.00ng

response 530331

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.19
183.00	11.60	12.18
0.00	0.00	0.00