

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF012318\
 Data File : BF102376.D
 Acq On : 24 Jan 2018 7:57
 Operator : SJ/JU
 Sample : J1214-01DL 4X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-PH3-MGP-01DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.887	473	476	482	rBV	36053	40244	3.46%	0.209%
2	5.316	545	549	561	rBV	677097	675607	58.13%	3.505%
3	6.345	721	724	738	rBV	708017	735089	63.25%	3.813%
4	6.481	743	747	754	rBV	898333	749295	64.48%	3.887%
5	6.710	783	786	794	rBV	810060	781967	67.29%	4.056%
6	6.869	809	813	816	rBV	471175	442962	38.12%	2.298%
7	7.275	878	882	893	rBV	442691	414621	35.68%	2.151%
8	7.739	957	961	965	rBV4	16908	20622	1.77%	0.107%
9	7.998	1001	1005	1007	rBV	1172634	1122110	96.56%	5.821%
10	8.016	1007	1008	1016	rVB	664965	458455	39.45%	2.378%
11	8.557	1094	1100	1103	rBV	23983	28353	2.44%	0.147%
12	8.710	1123	1126	1133	rBV	184927	162373	13.97%	0.842%
13	8.804	1139	1142	1150	rVB	310543	304669	26.22%	1.580%
14	9.069	1184	1187	1192	rBV	635623	508747	43.78%	2.639%
15	9.175	1202	1205	1211	rVB	103928	100134	8.62%	0.519%
16	9.269	1215	1221	1227	rVB2	35572	50708	4.36%	0.263%
17	9.339	1228	1233	1236	rBV2	94281	125524	10.80%	0.651%
18	9.410	1241	1245	1247	rVV	139539	145886	12.55%	0.757%
19	9.433	1247	1249	1252	rVV	78391	73716	6.34%	0.382%
20	9.469	1252	1255	1259	rVV2	88962	89785	7.73%	0.466%
21	9.522	1262	1264	1269	rVV	70831	74803	6.44%	0.388%
22	9.610	1276	1279	1284	rBV	327854	272900	23.48%	1.416%
23	9.751	1295	1303	1306	rBV	1208040	1162142	100.00%	6.028%
24	9.780	1306	1308	1317	rVV2	123194	134793	11.60%	0.699%
25	9.851	1317	1320	1324	rVV2	19457	23439	2.02%	0.122%
26	9.951	1334	1337	1341	rVV2	54002	50581	4.35%	0.262%
27	9.992	1341	1344	1348	rVB	31348	29505	2.54%	0.153%
28	10.063	1353	1356	1359	rBV	39038	40891	3.52%	0.212%
29	10.151	1367	1371	1373	rBV2	35914	45014	3.87%	0.233%
30	10.169	1373	1374	1377	rVB3	23674	18042	1.55%	0.094%
31	10.198	1377	1379	1382	rBV	41150	35858	3.09%	0.186%
32	10.298	1392	1396	1401	rVB	317710	318999	27.45%	1.655%
33	10.463	1419	1424	1427	rVB2	56990	60359	5.19%	0.313%
34	10.533	1431	1436	1442	rBV2	359192	453082	38.99%	2.350%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF012318\
 Data File : BF102376.D
 Acq On : 24 Jan 2018 7:57
 Operator : SJ/JU
 Sample : J1214-01DL 4X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-PH3-MGP-01DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.663	1454	1458	1464	rVB2	39125	48580	4.18%	0.252%
36	10.845	1484	1489	1491	rBV2	67918	89546	7.71%	0.464%
37	10.869	1491	1493	1497	rVV	52547	48709	4.19%	0.253%
38	10.927	1500	1503	1506	rVB	42362	36699	3.16%	0.190%
39	10.975	1506	1511	1512	rBV5	15192	18490	1.59%	0.096%
40	10.992	1512	1514	1516	rVV3	23031	21740	1.87%	0.113%
41	11.045	1520	1523	1526	rVV	30858	30285	2.61%	0.157%
42	11.080	1526	1529	1533	rVV6	13529	20948	1.80%	0.109%
43	11.127	1533	1537	1542	rVB	80297	89905	7.74%	0.466%
44	11.233	1552	1555	1557	rBV	1080479	964260	82.97%	5.002%
45	11.257	1557	1559	1564	rVV	1318735	1056052	90.87%	5.478%
46	11.310	1564	1568	1572	rVV	777089	674845	58.07%	3.501%
47	11.345	1572	1574	1576	rVV	34459	36268	3.12%	0.188%
48	11.392	1579	1582	1588	rVV6	23297	36621	3.15%	0.190%
49	11.475	1592	1596	1598	rBV4	18766	26606	2.29%	0.138%
50	11.527	1602	1605	1608	rVV	57383	49239	4.24%	0.255%
51	11.563	1609	1611	1616	rVB2	28881	34494	2.97%	0.179%
52	11.733	1637	1640	1643	rBV	173859	155484	13.38%	0.807%
53	11.763	1643	1645	1649	rVV	156797	127571	10.98%	0.662%
54	11.810	1650	1653	1656	rVV	75217	71574	6.16%	0.371%
55	11.845	1656	1659	1661	rVV	276781	268634	23.12%	1.393%
56	11.869	1661	1663	1669	rVB	109693	96148	8.27%	0.499%
57	12.027	1687	1690	1694	rVB	94036	88719	7.63%	0.460%
58	12.210	1718	1721	1723	rBV	26110	18782	1.62%	0.097%
59	12.280	1729	1733	1736	rBV	73823	72503	6.24%	0.376%
60	12.322	1736	1740	1742	rVV2	48459	63563	5.47%	0.330%
61	12.374	1745	1749	1753	rVV3	21479	39108	3.37%	0.203%
62	12.445	1757	1761	1766	rBV	596538	519534	44.70%	2.695%
63	12.539	1774	1777	1781	rVB	84614	71480	6.15%	0.371%
64	12.674	1795	1800	1806	rVV	663252	646994	55.67%	3.356%
65	12.727	1806	1809	1813	rVB3	17775	22262	1.92%	0.115%
66	12.816	1820	1824	1831	rVB	411057	359797	30.96%	1.866%
67	12.892	1831	1837	1844	rVB4	36530	56445	4.86%	0.293%
68	12.980	1848	1852	1853	rVV2	38144	42585	3.66%	0.221%
69	12.998	1853	1855	1859	rVV2	89139	81417	7.01%	0.422%
70	13.069	1859	1867	1870	rVV	85124	89022	7.66%	0.462%
71	13.104	1870	1873	1877	rVV	59858	56060	4.82%	0.291%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF012318\
 Data File : BF102376.D
 Acq On : 24 Jan 2018 7:57
 Operator : SJ/JU
 Sample : J1214-01DL 4X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-PH3-MGP-01DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.169	1881	1884	1887	rVV2	39633	51570	4.44%	0.268%
73	13.198	1887	1889	1891	rVV2	44907	38776	3.34%	0.201%
74	13.227	1891	1894	1902	rVB	49100	54725	4.71%	0.284%
75	13.645	1963	1965	1967	rVV	40735	35007	3.01%	0.182%
76	13.668	1967	1969	1972	rVV	45750	39798	3.42%	0.206%
77	13.716	1975	1977	1985	rVB6	26415	37804	3.25%	0.196%
78	13.868	1998	2003	2006	rBV2	878620	980932	84.41%	5.088%
79	13.892	2006	2007	2016	rVV	175011	163534	14.07%	0.848%
80	13.974	2016	2021	2023	rVV2	23812	29629	2.55%	0.154%
81	14.015	2026	2028	2037	rVB3	22522	40789	3.51%	0.212%
82	14.257	2065	2069	2072	rVV	38118	48419	4.17%	0.251%
83	14.286	2072	2074	2079	rVV	19944	20328	1.75%	0.105%
84	14.351	2079	2085	2088	rVV4	29519	47873	4.12%	0.248%
85	14.380	2088	2090	2092	rVV2	29259	28427	2.45%	0.147%
86	14.404	2092	2094	2100	rVV3	37307	47743	4.11%	0.248%
87	14.886	2172	2176	2185	rBV	98334	205966	17.72%	1.068%
88	14.957	2185	2188	2191	rVV2	26789	30423	2.62%	0.158%
89	14.992	2191	2194	2197	rVB	26594	29432	2.53%	0.153%
90	15.174	2220	2225	2231	rBV	78856	98998	8.52%	0.514%
91	15.233	2231	2235	2240	rBV	129186	153876	13.24%	0.798%
92	15.292	2240	2245	2252	rBV	546506	737581	63.47%	3.826%
93	15.715	2313	2317	2324	rBV3	31106	55547	4.78%	0.288%
94	15.821	2332	2335	2341	rBV6	19700	37814	3.25%	0.196%
95	16.192	2391	2398	2405	rBV3	27983	60153	5.18%	0.312%
96	16.674	2475	2480	2488	rBV2	35301	72463	6.24%	0.376%
97	16.745	2488	2492	2499	rVB6	20425	41930	3.61%	0.218%
98	17.098	2546	2552	2560	rBV2	29843	64373	5.54%	0.334%
99	17.321	2586	2590	2595	rBV3	11254	20373	1.75%	0.106%
100	17.398	2599	2603	2609	rVV7	10277	21481	1.85%	0.111%


Sum of corrected areas: 19278008

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_F\DATA\BF012318\
Data File : BF102376.D
Acq On : 24 Jan 2018 7:57
Operator : SJ/JU
Sample : J1214-01DL 4X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-PH3-MGP-01DL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

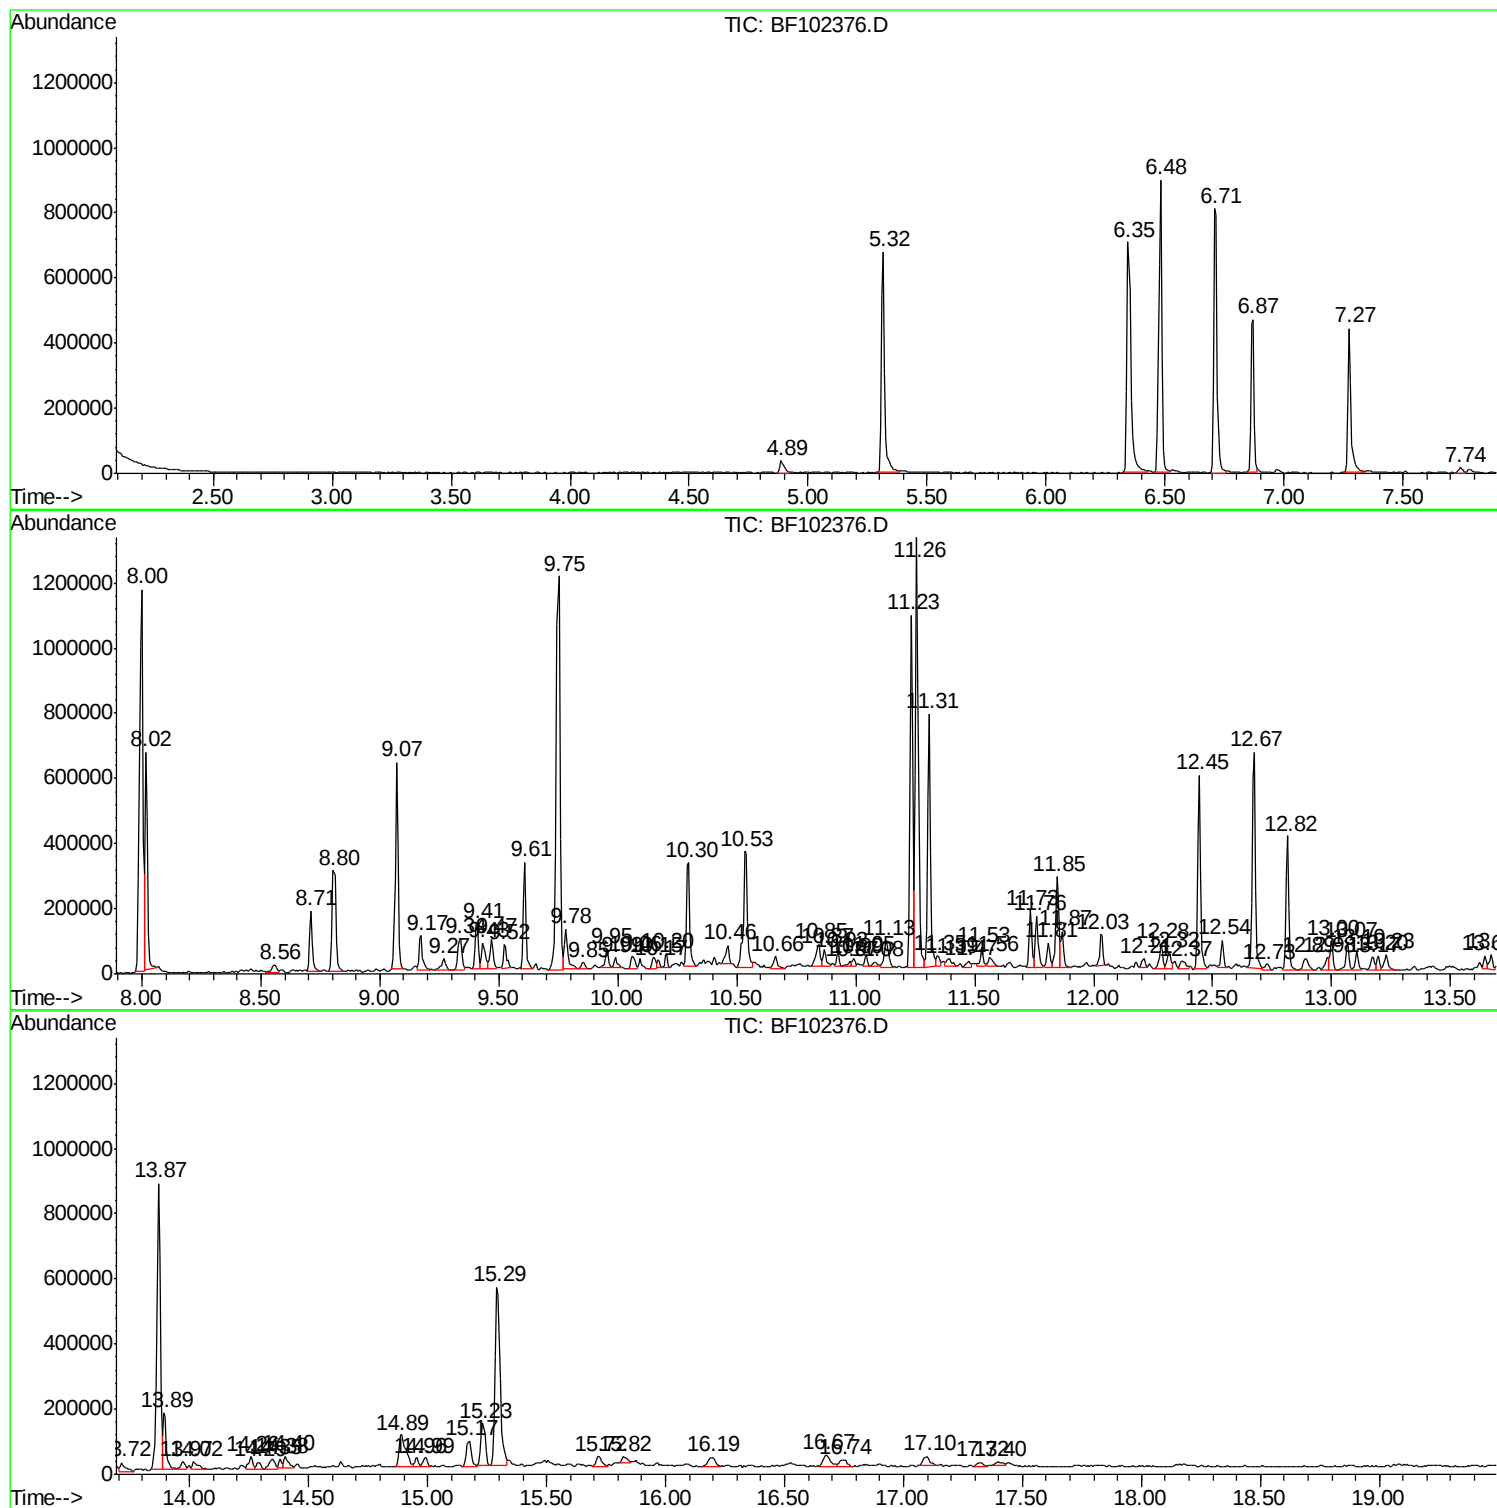

DbaaaPath::\\X740028001700SV00ASRVNRPBHM1BNAFNDATAAB0022388\
 DbaaaFile::BBE002306DD
 AcqQOn :24Jan2008 77537
 Operator::SSJU
 Sample::J1221400DL4X
 Misc :
 ASSVal :288 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 WC-PH3-MGP-01DL

QcAntMebdd::ZZ\NRPBHM1BNAFMEH00S8200BB002228MM
 QcAntFile::ASBPBNASSANDABBSF00R55P000NTC6ALBRATION

TICLibrary :CC\DATAABASENOSTI11LL
 TICIntegratIonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
