


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_F\Data\BF012318\
Data File : BF102333.D
Acq On : 23 Jan 2018 9:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 23 00:43:41 2018

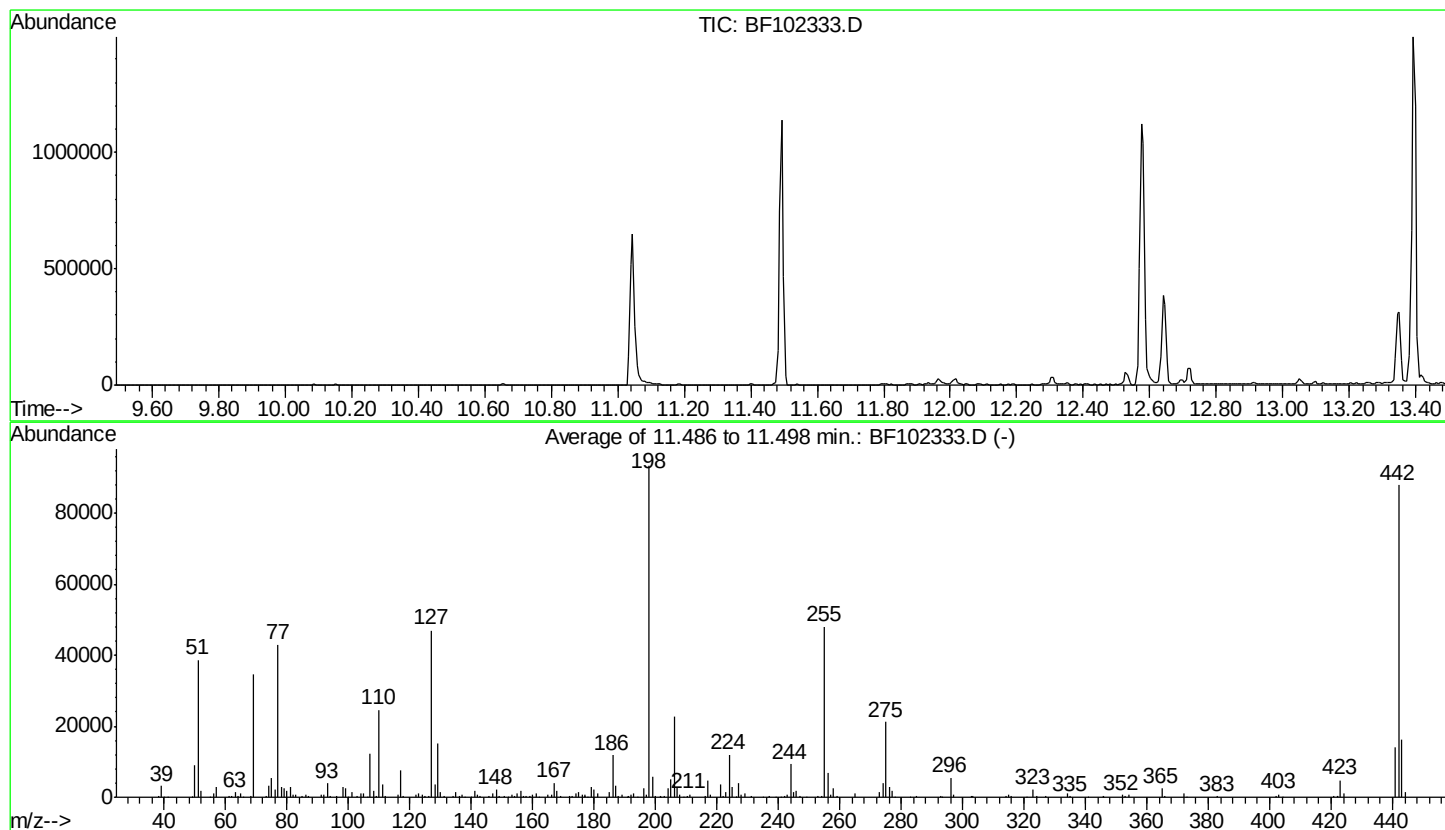

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	38631	PASS
68	69	0.00	2	1.4	485	PASS
69	198	0.00	100	36.9	34456	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	47034	PASS
197	198	0.00	2	0.6	587	PASS
198	198	100	100	100.0	93349	PASS
199	198	5	9	6.2	5805	PASS
275	198	10	60	22.6	21111	PASS
365	198	1	100	2.7	2504	PASS
441	443	0.01	100	86.7	14191	PASS
442	198	50	100	94.0	87789	PASS
443	442	15	24	18.6	16363	PASS