


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_F\Data\BF012318\
 Data File : BF102347.D
 Acq On : 23 Jan 2018 17:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 23 00:43:41 2018

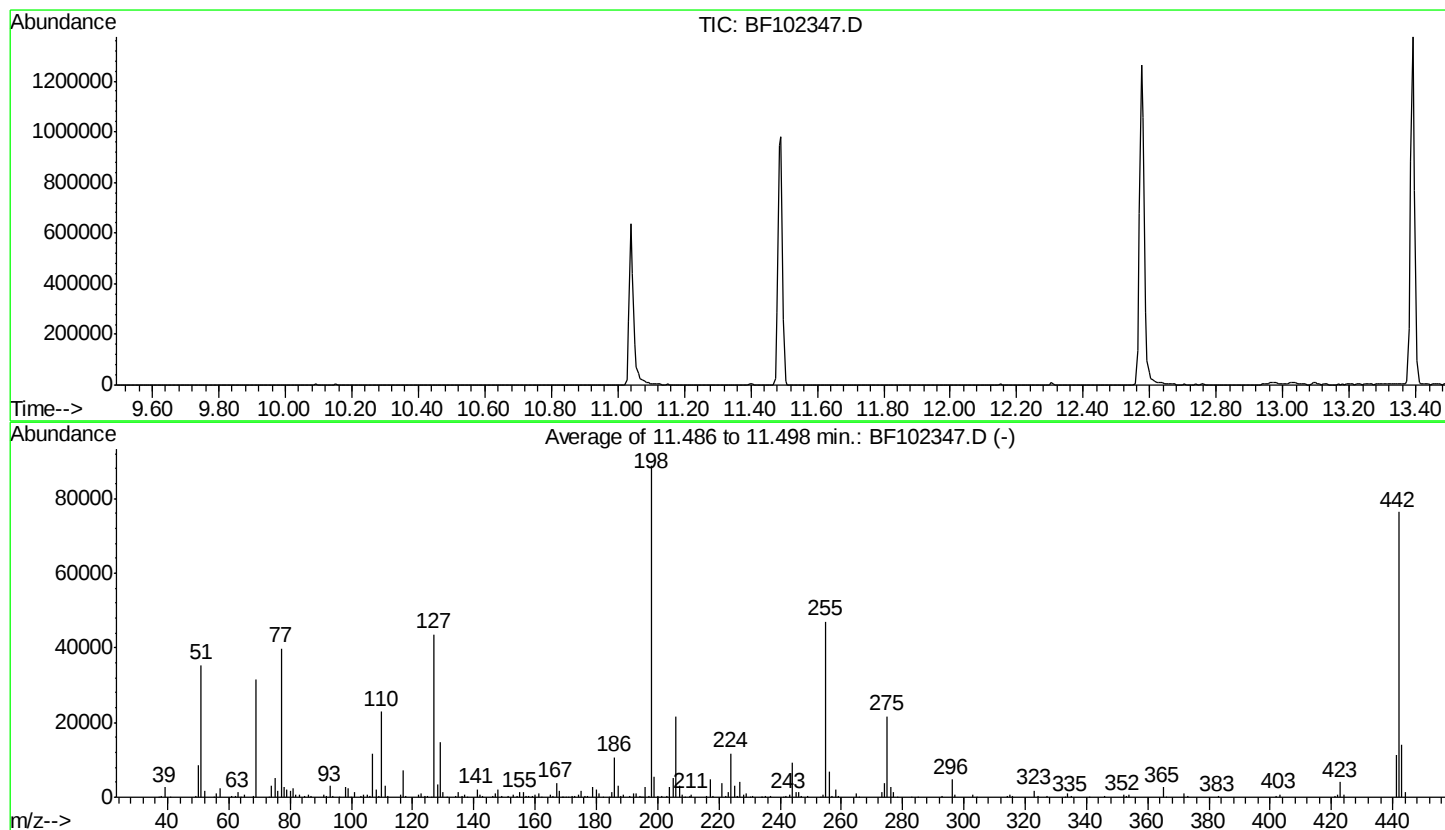

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	35413	PASS
68	69	0.00	2	1.6	491	PASS
69	198	0.00	100	35.6	31580	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	43645	PASS
197	198	0.00	2	0.6	494	PASS
198	198	100	100	100.0	88829	PASS
199	198	5	9	6.3	5570	PASS
275	198	10	60	24.3	21605	PASS
365	198	1	100	3.0	2669	PASS
441	443	0.01	100	80.9	11381	PASS
442	198	50	100	85.9	76328	PASS
443	442	15	24	18.4	14064	PASS