


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_F\Data\BF012318\
 Data File : BF102374.D
 Acq On : 24 Jan 2018 6:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 23 00:43:41 2018

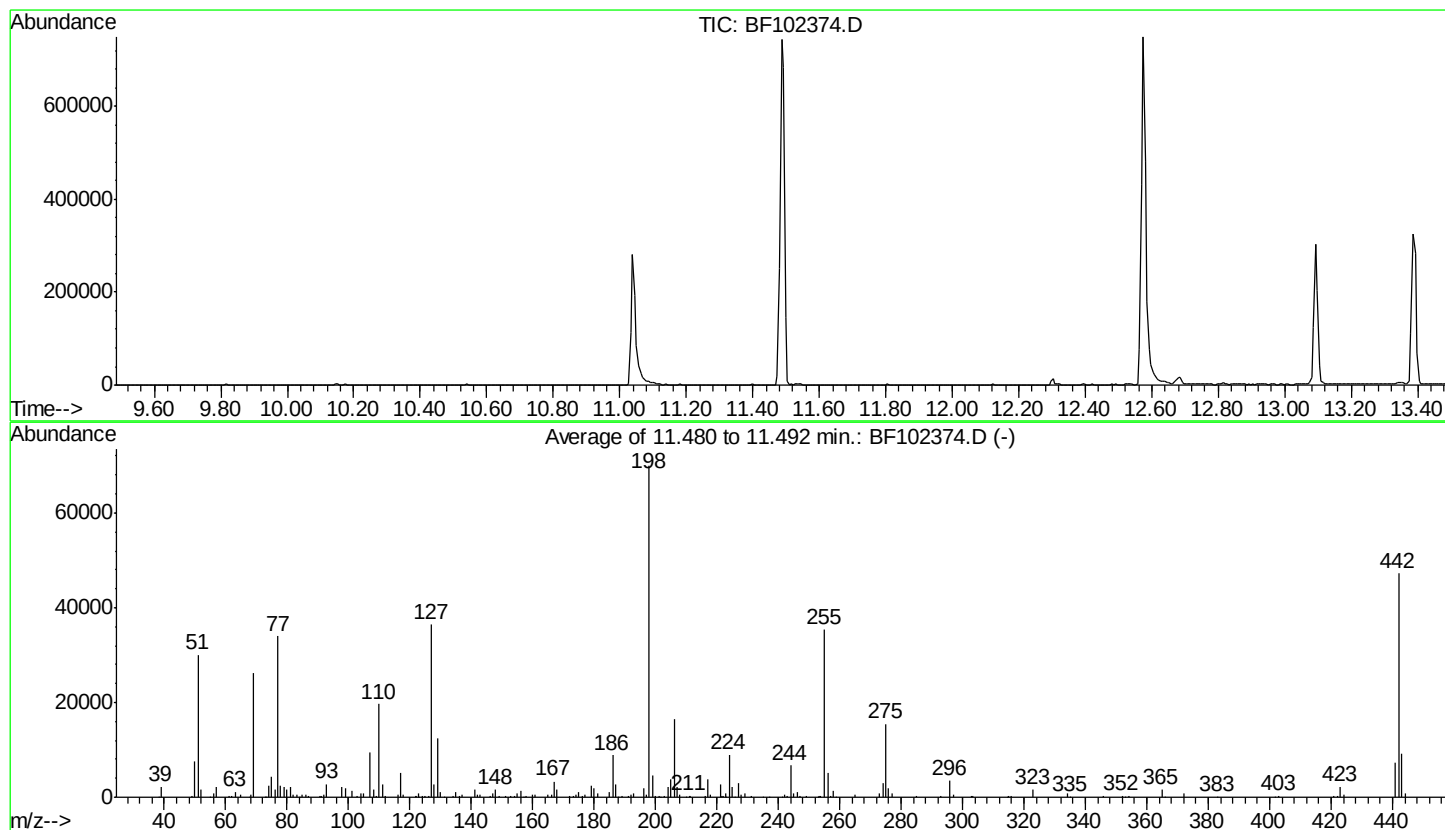

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	30002	PASS
68	69	0.00	2	1.6	428	PASS
69	198	0.00	100	37.4	26168	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.1	36429	PASS
197	198	0.00	2	0.8	591	PASS
198	198	100	100	100.0	69976	PASS
199	198	5	9	6.4	4506	PASS
275	198	10	60	22.1	15486	PASS
365	198	1	100	2.2	1563	PASS
441	443	0.01	100	80.1	7272	PASS
442	198	50	100	67.5	47228	PASS
443	442	15	24	19.2	9083	PASS