
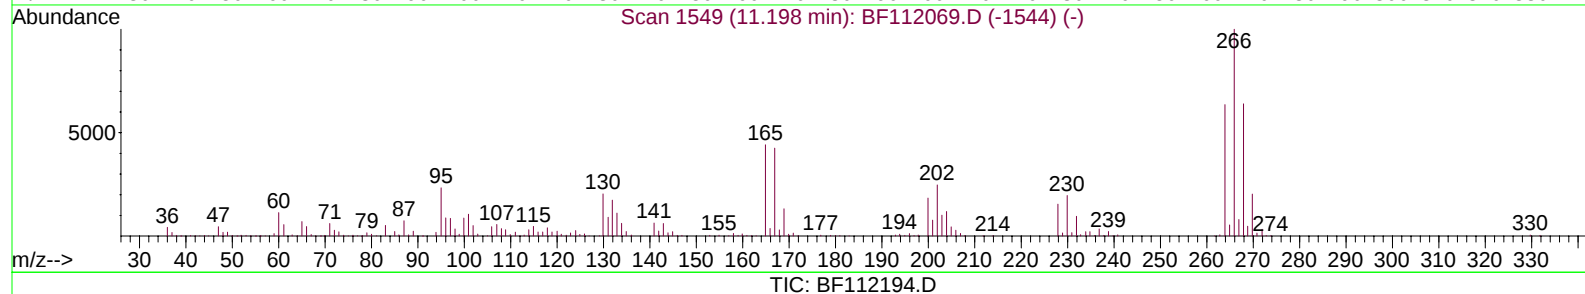
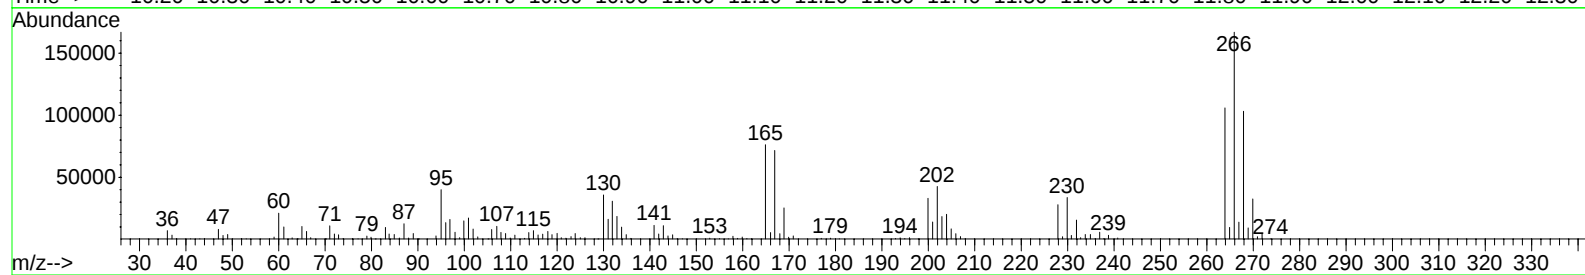


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012319\
Data File : BF112194.D
Acq On : 23 Jan 2019 11:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 17:57:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 19 01:02:12 2019
Response via : Initial Calibration

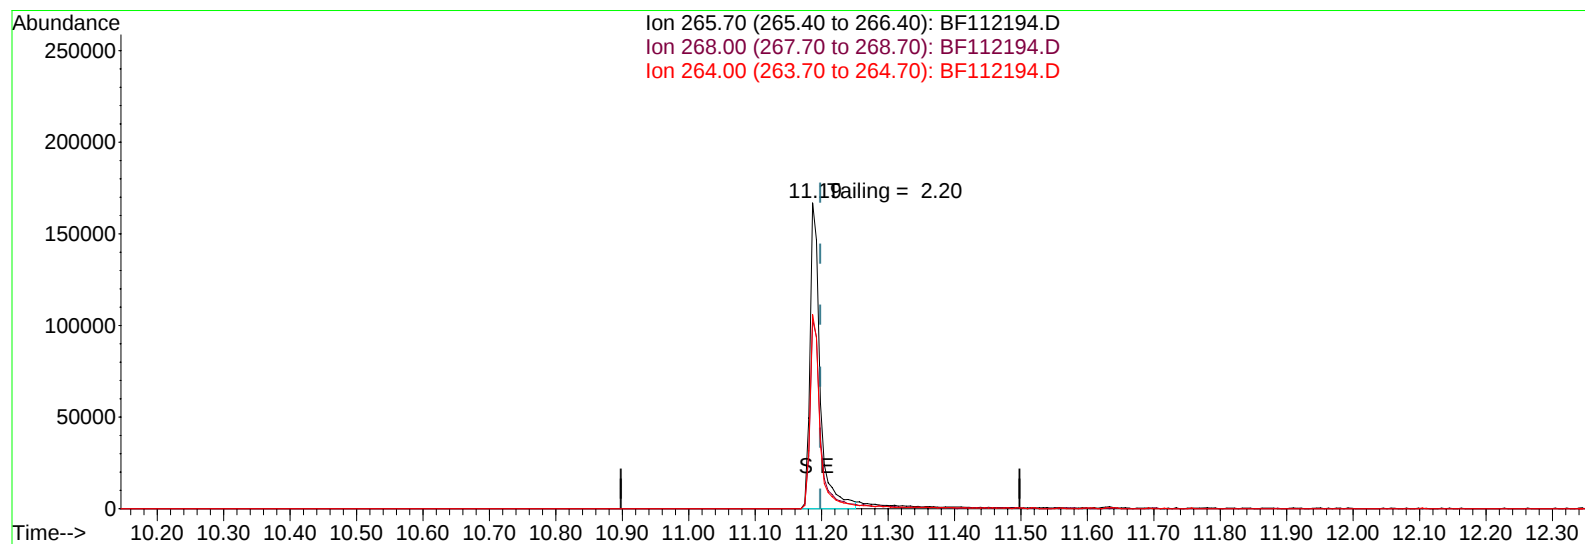

(70) Pentachlorophenol (C)




11.186min (-0.012) 84068.89ng

response 189983

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	61.83
264.00	63.60	63.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012319\
 Data File : BF112194.D
 Acq On : 23 Jan 2019 11:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 17:57:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 19 01:02:12 2019
 Response via : Initial Calibration

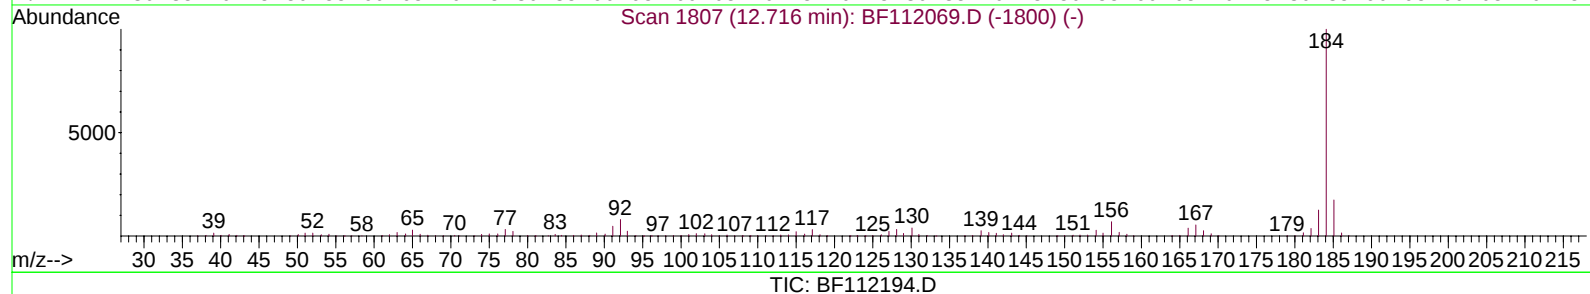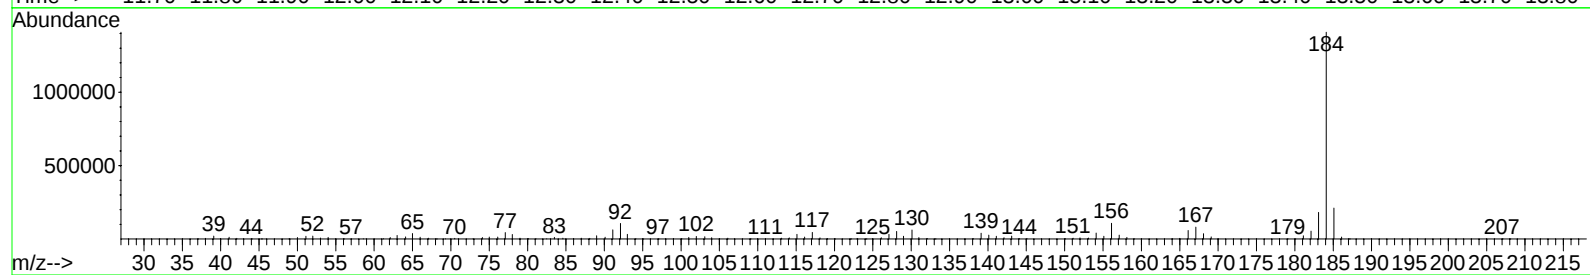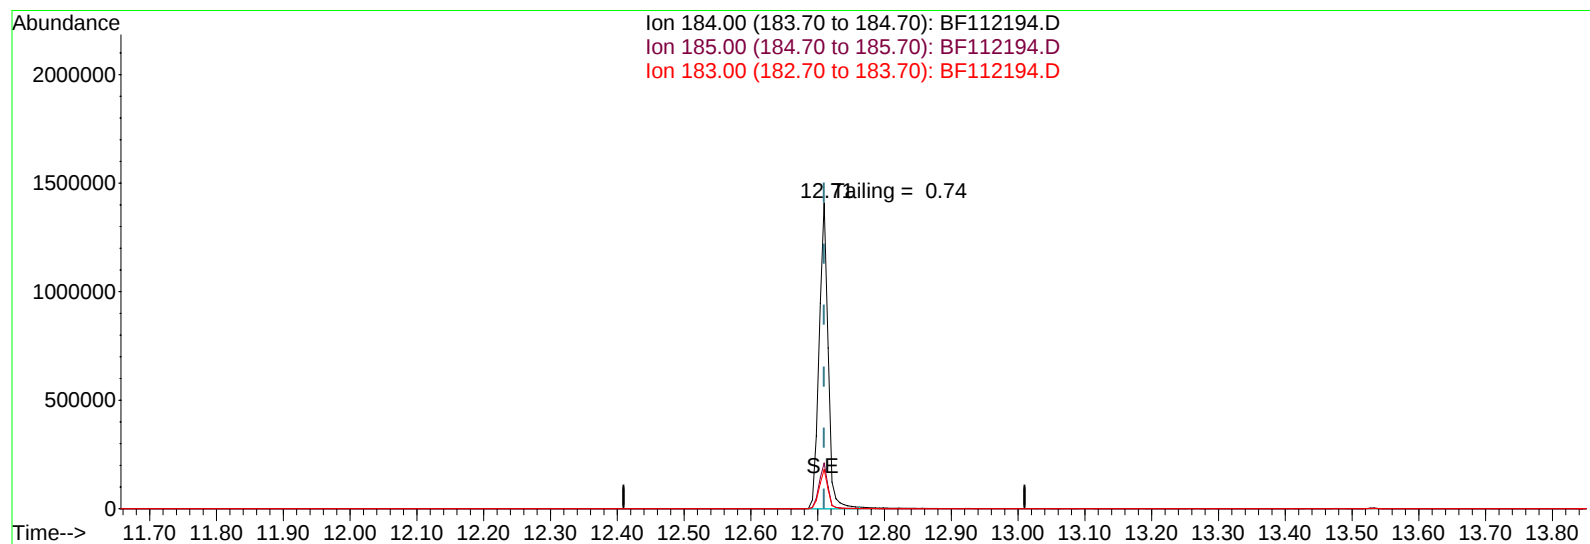

(77) Benzidine

12.710min (+0.000) 57831.37ng

response 1333318

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.98
183.00	12.50	12.85
0.00	0.00	0.00