
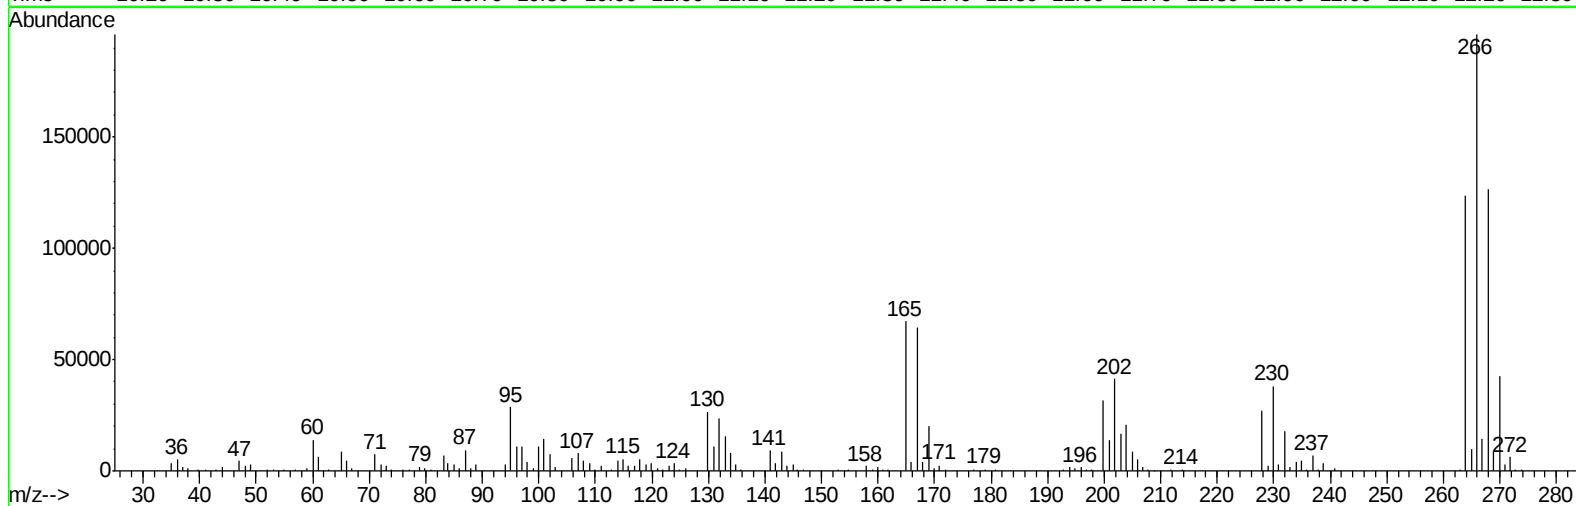


Data File : BF118676.D  
Acq On : 23 Jan 2020 14:48  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 03:28:24 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 20 14:45:03 2020  
Response via : Initial Calibration

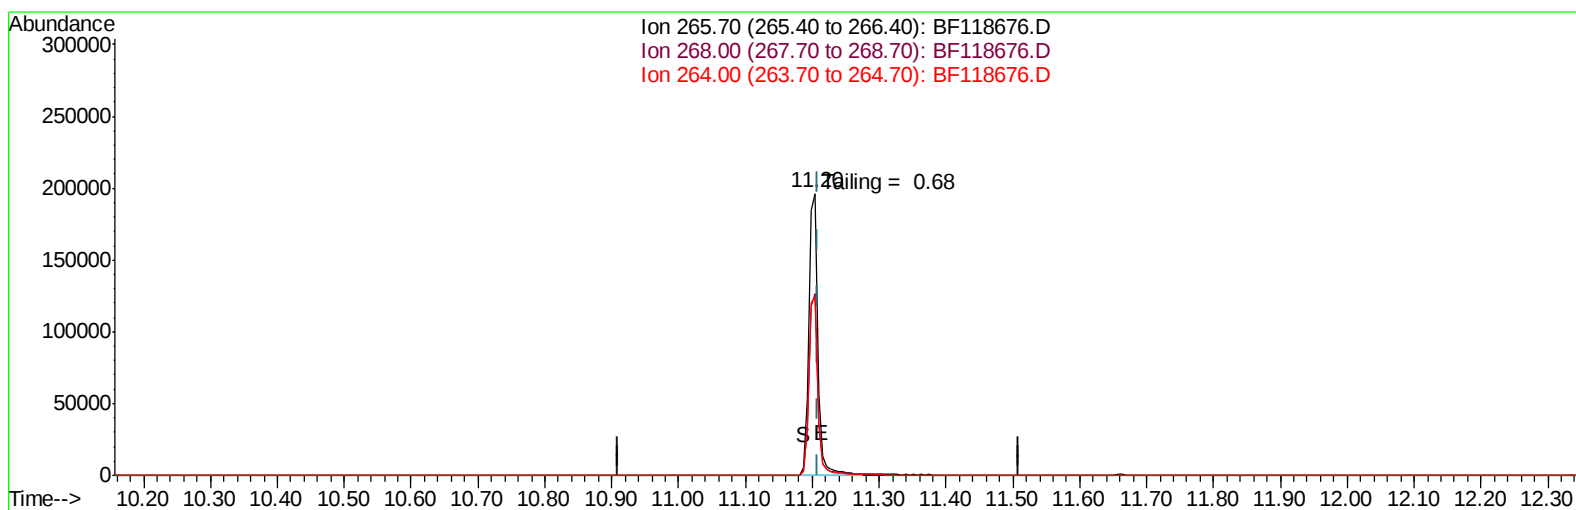

TIC: BF118676.D

(70) Pentachlorophenol (C)



11.204min (-0.006) 24397.15ng m

response 189426

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.10 | 64.52 |
| 264.00 | 65.50 | 62.98 |
| 0.00   | 0.00  | 0.00  |

Data File : BF118676.D  
Acq On : 23 Jan 2020 14:48  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 03:28:24 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jan 20 14:45:03 2020  
Response via : Initial Calibration

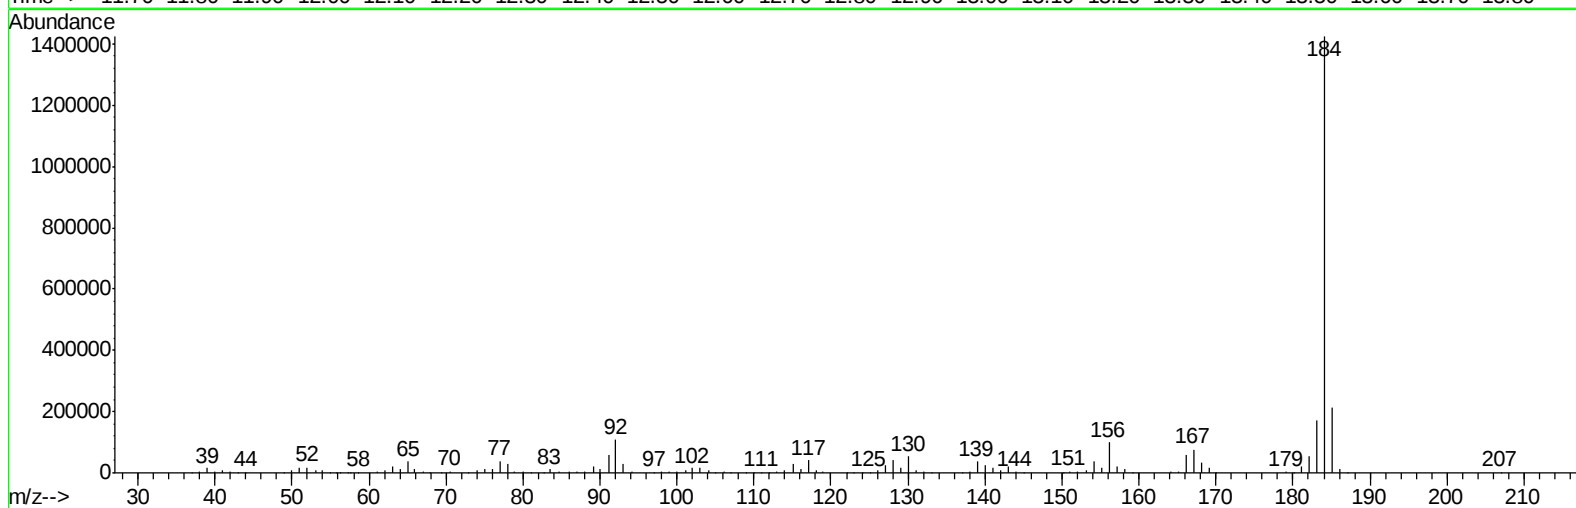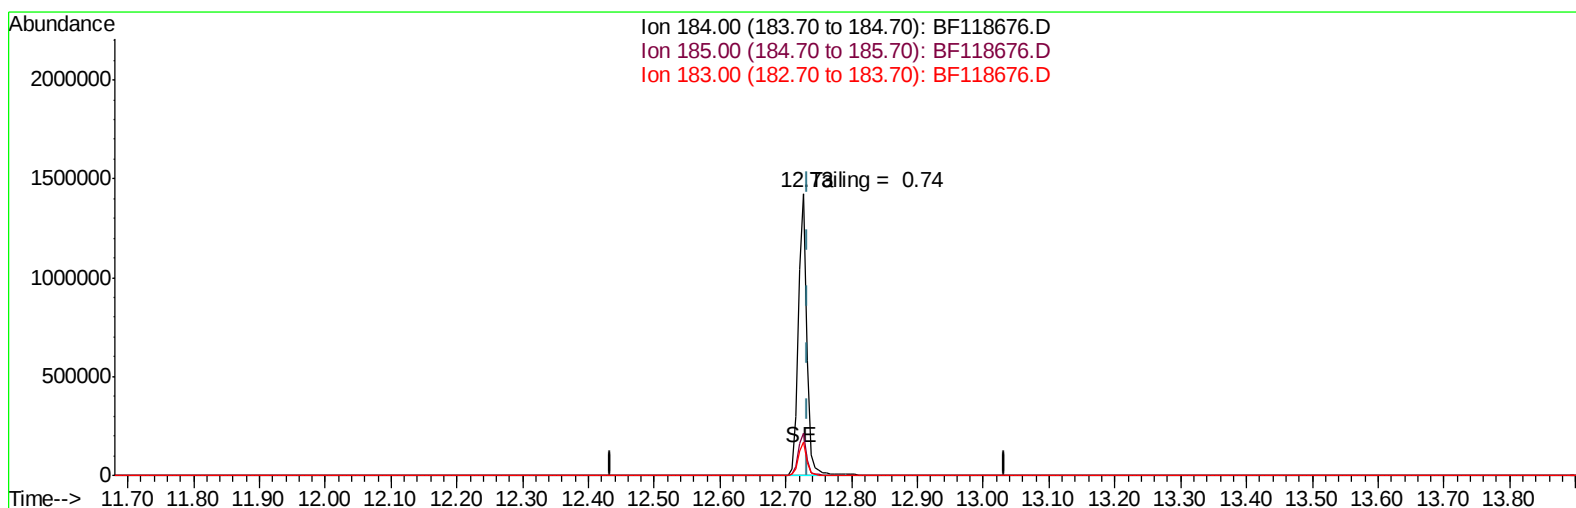

TIC: BF118676.D

(77) Benzidine

12.727min (-0.006) 0.00ng

response 1287357

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.10 | 14.86 |
| 183.00 | 12.00 | 12.04 |
| 0.00   | 0.00  | 0.00  |