


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012320\
 Data File : BF118676.D
 Acq On : 23 Jan 2020 14:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 27 14:24:10 2020

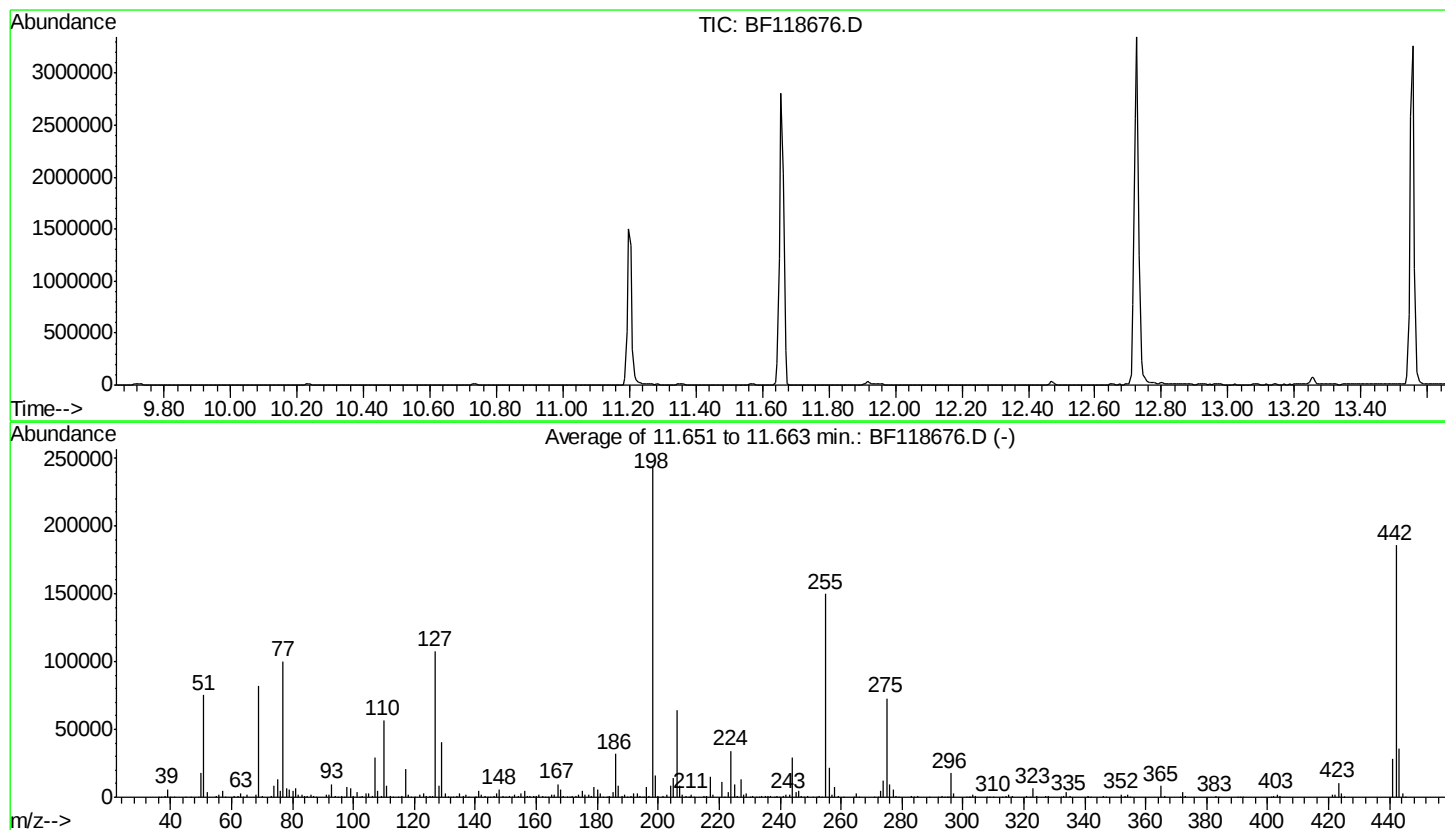

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	75314	PASS
68	69	0.00	2	1.8	1503	PASS
69	198	0.00	100	33.4	81706	PASS
70	69	0.00	2	0.7	545	PASS
127	198	10	80	43.9	107352	PASS
197	198	0.00	2	0.5	1251	PASS
198	198	100	100	100.0	244330	PASS
199	198	5	9	6.6	16062	PASS
275	198	10	60	29.8	72872	PASS
365	198	1	100	3.3	8139	PASS
441	198	0.01	100	11.8	28783	PASS
442	198	50	100	75.9	185400	PASS
443	442	15	24	19.5	36080	PASS